

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
 Data File : VW023232.D
 Acq On : 21 May 2022 05:25
 Operator : SY/VA
 Sample : N2926-07
 Misc : 4.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY16

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 21 06:03:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 21 01:30:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	9999	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	10126	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	2089	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	4286	20.893	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.560%
7) Chloroethane-d5	2.897	69	2895	21.691	ug/L	0.02
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.760%
11) 1,1-Dichloroethene-d2	4.031	63	4536	17.112	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.440%
21) 2-Butanone-d5	7.104	46	1421m	36.432	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.860%
24) Chloroform-d	7.659	84	8225	28.077	ug/L	0.01
Spiked Amount	25.000	Range	40 - 150	Recovery	=	112.320%
26) 1,2-Dichloroethane-d4	8.311	65	5118	31.854	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	127.400%
32) Benzene-d6	8.275	84	14289	24.482	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.920%
36) 1,2-Dichloropropane-d6	9.280	67	4673	28.502	ug/L	0.01
Spiked Amount	25.000	Range	70 - 120	Recovery	=	114.000%
41) Toluene-d8	10.323	98	10768	19.098	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.400%
43) trans-1,3-Dichloroprop...	10.579	79	1054	13.962	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	55.840%
47) 2-Hexanone-d5	0.000	63	0d	0.000	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.000%#
56) 1,1,2,2-Tetrachloroeth...	12.695	84	3019	19.756	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	1787	24.471	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.880%
Target Compounds						Qvalue
15) Methyl Acetate	4.678	43	8623	146.982	ug/L	# 68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052022\
Data File : VW023232.D
Acq On : 21 May 2022 05:25
Operator : SY/VA
Sample : N2926-07
Misc : 4.30g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EXY16

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/22/2022
Supervised By : Mahesh Dadoda 05/25/2022


Quant Time: May 21 06:03:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 21 01:30:17 2022
Response via : Initial Calibration

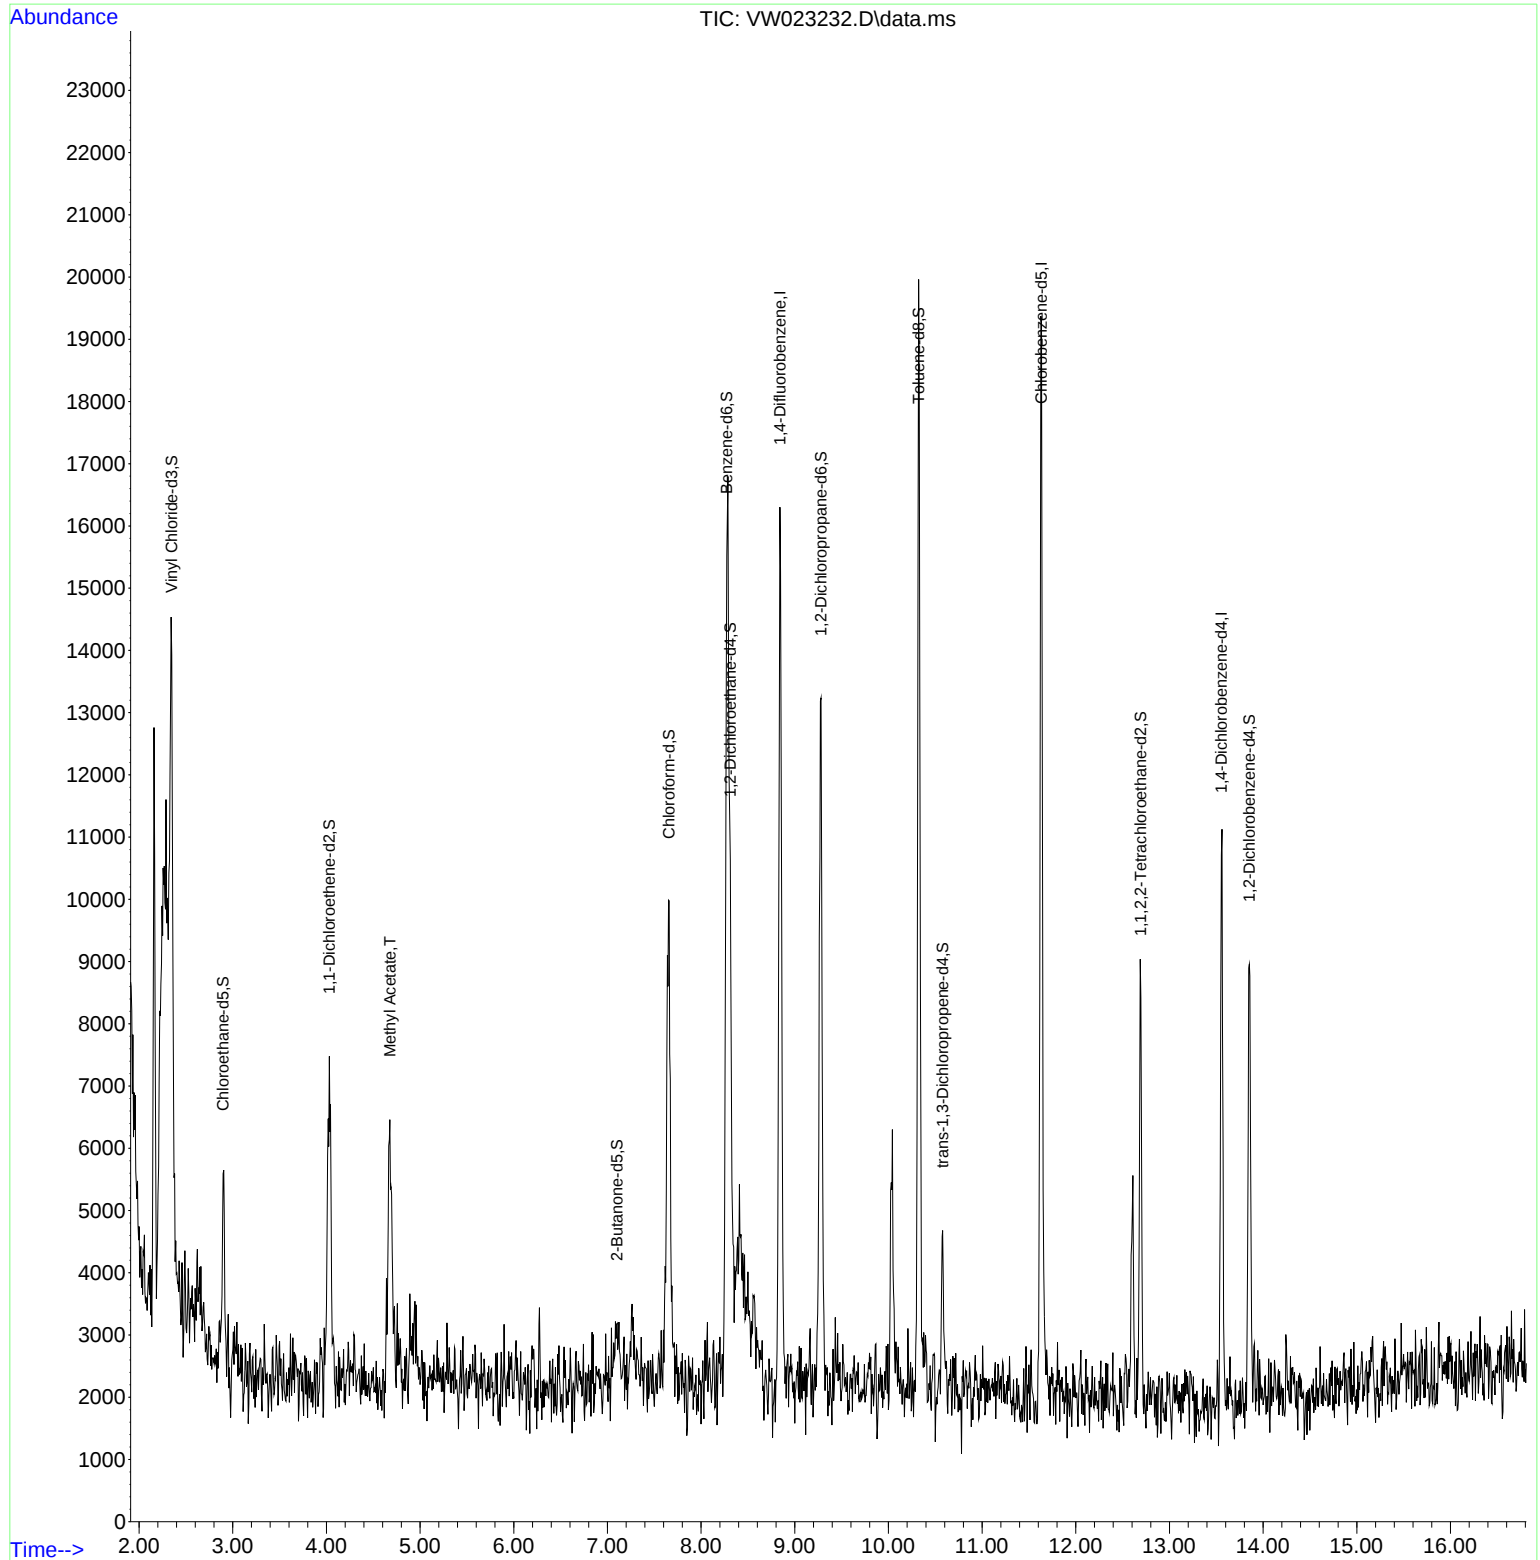

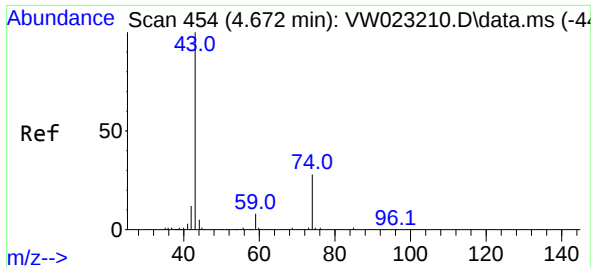

#15
Methyl Acetate
Concen: 146.982 ug/L
RT: 4.678 min Scan# 41
Delta R.T. 0.006 min
Lab File: VW023232.D
Acq: 21 May 2022 05:25

Instrument :
MSVOA_W
ClientSampleId :
EXY16

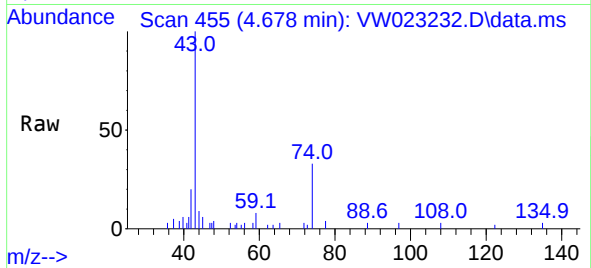

Tgt Ion: 43 Resp: 862
Ion Ratio Lower Upper
43 100
74 10.7 21.9 32.9

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/22/2022
Supervised By :Mahesh Dadoda 05/25/2022

