

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052224\
 Data File : VW028675.D
 Acq On : 22 May 2024 10:02
 Operator : SY/MD
 Sample : P2548-16
 Misc : 5.50g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 BH611

Manual IntegrationsAPPROVED

Quant Time: May 23 00:21:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 23 00:20:47 2024
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

05/23/2024
 Supervised By :Mahesh
 Dadoda

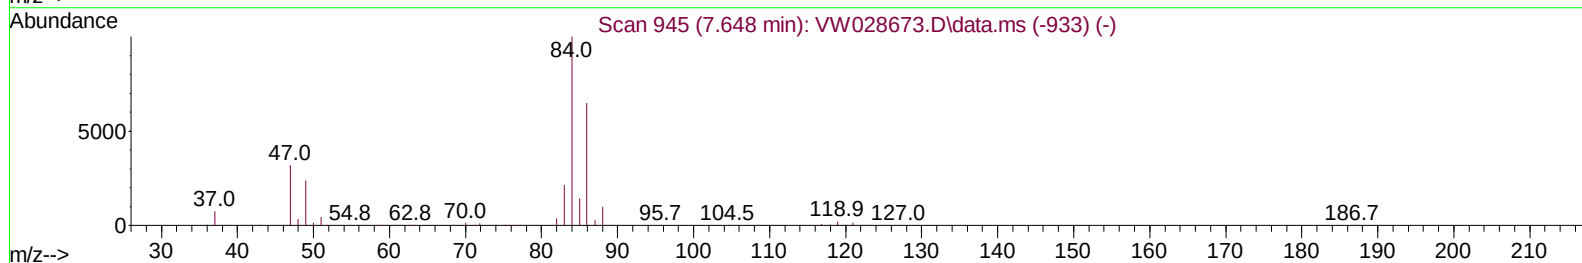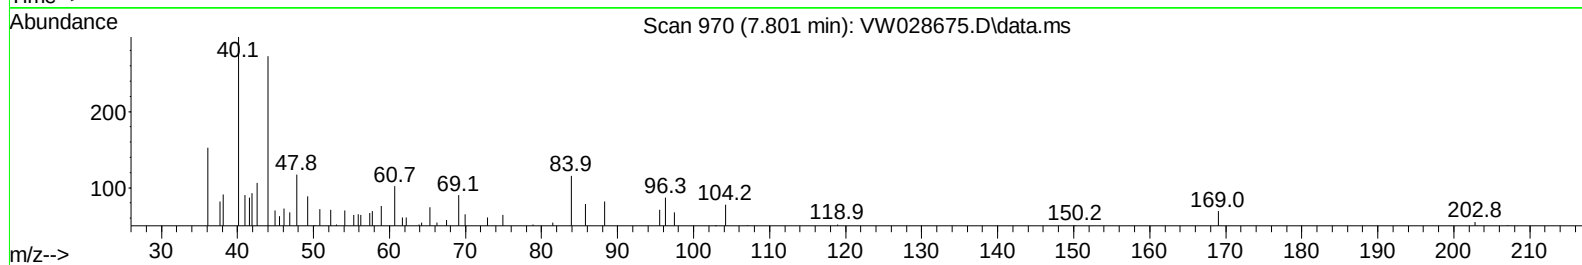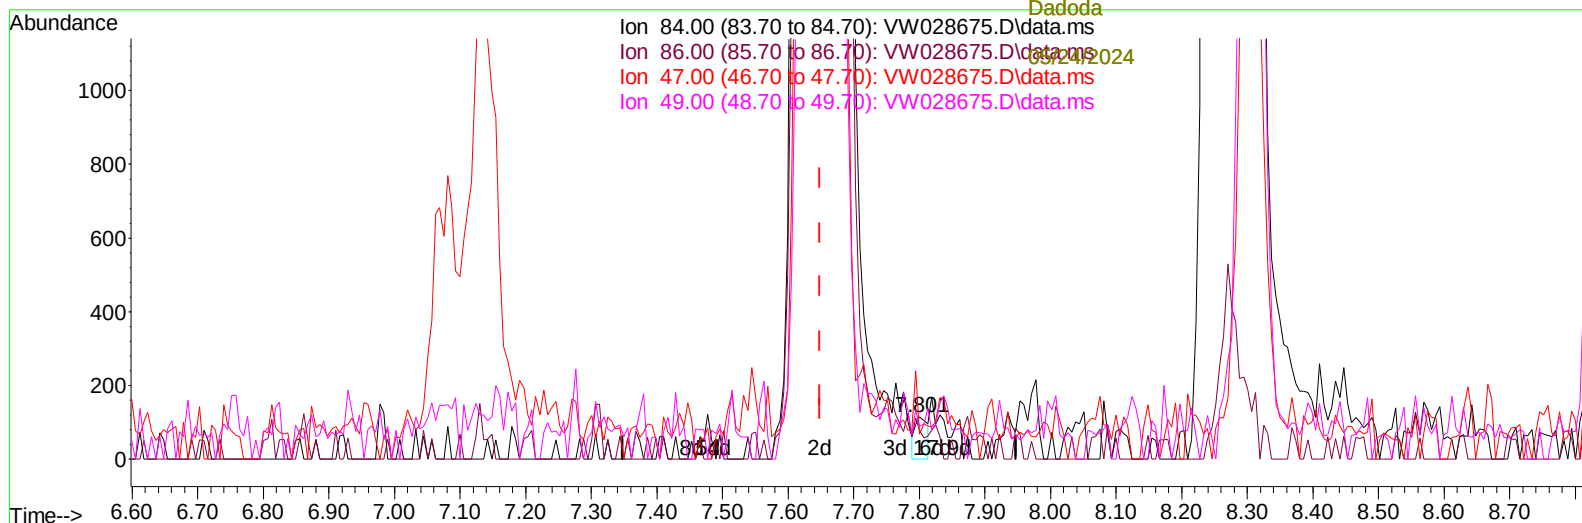

TIC: VW028675.D\data.ms

(24) Chloroform-d (S)

7.801min (+ 0.152) 0.01 ug/L

response 151

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.40	60.26
47.00	49.80	41.72
49.00	28.30	32.45

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052224\
 Data File : VW028675.D
 Acq On : 22 May 2024 10:02
 Operator : SY/MD
 Sample : P2548-16
 Misc : 5.50g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 BH611

Manual IntegrationsAPPROVED

Quant Time: May 23 00:21:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 23 00:20:47 2024
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

05/23/2024
 Supervised By :Mahesh
 Dadoda

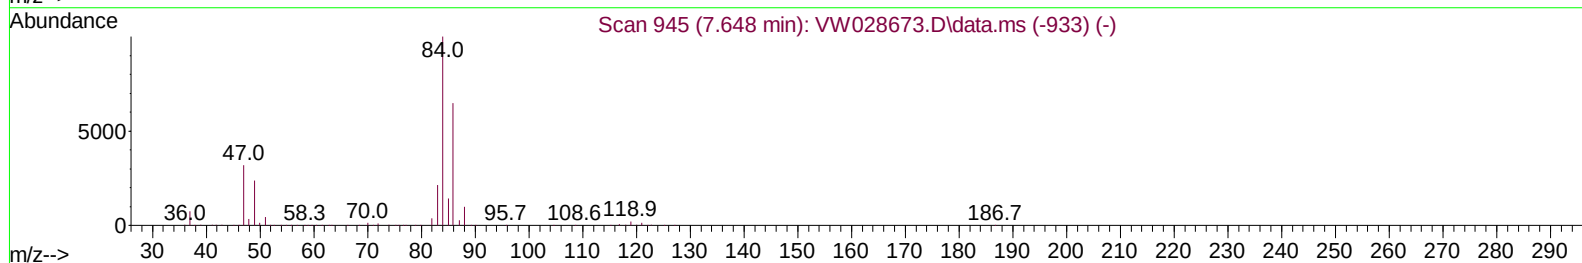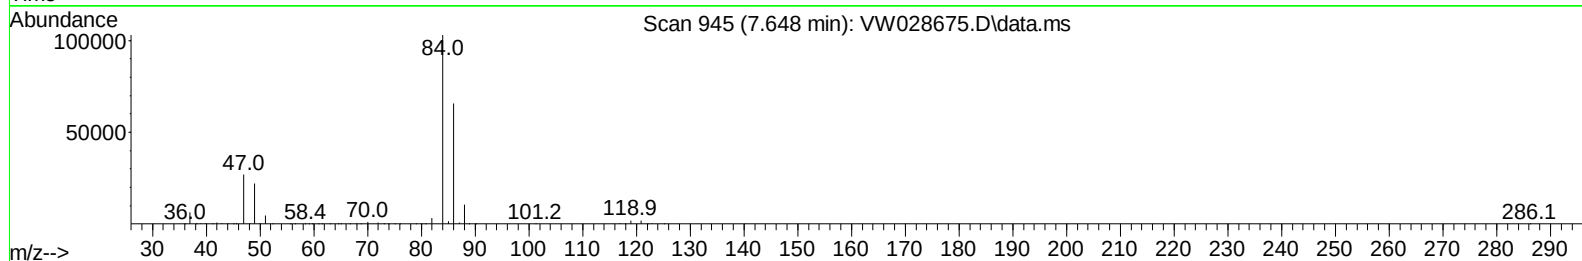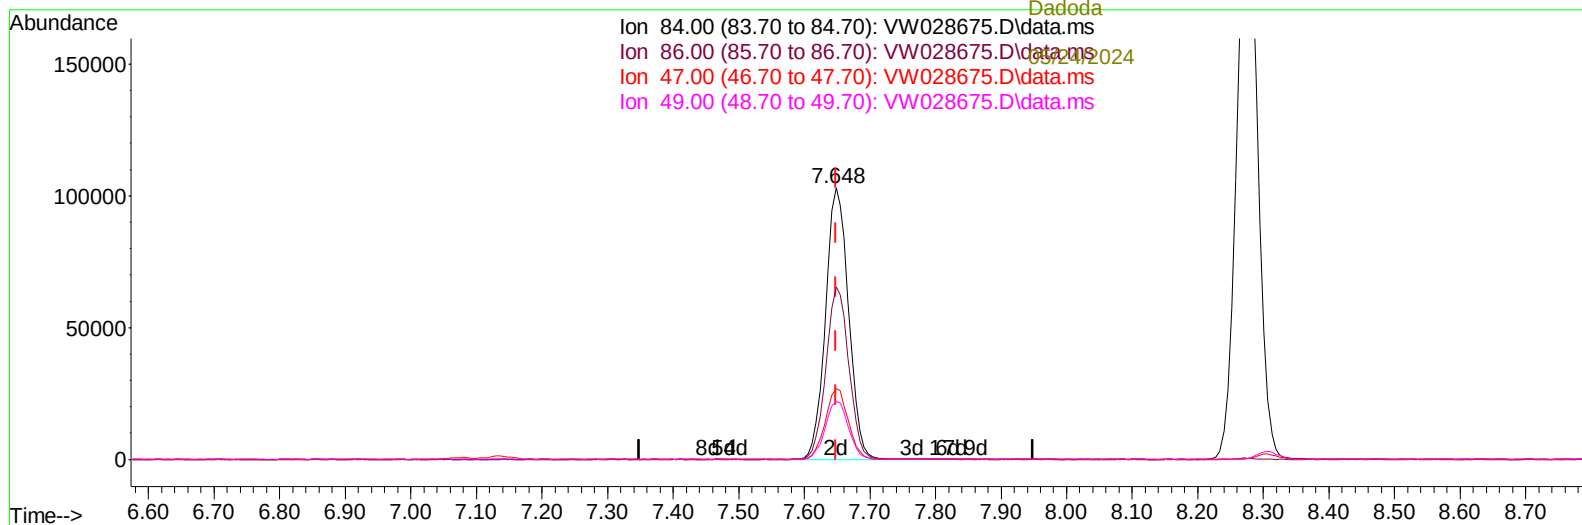

TIC: VW028675.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 18.63 ug/L m

response 251243

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.40	0.04#
47.00	49.80	0.03#
49.00	28.30	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052224\
Data File : VW028675.D
Acq On : 22 May 2024 10:02
Operator : SY/MD
Sample : P2548-16
Misc : 5.50g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH611


Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt


05/23/2024
Supervised By :Mahesh
Dadoda

Quant Time: May 23 00:21:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 23 00:20:47 2024
Response via : Initial Calibration


Ion 65.00 (64.70 to 65.70): VW028675.D\data.ms
Ion 67.00 (66.70 to 67.70): VW028675.D\data.ms
Ion 51.00 (50.70 to 51.70): VW028675.D\data.ms

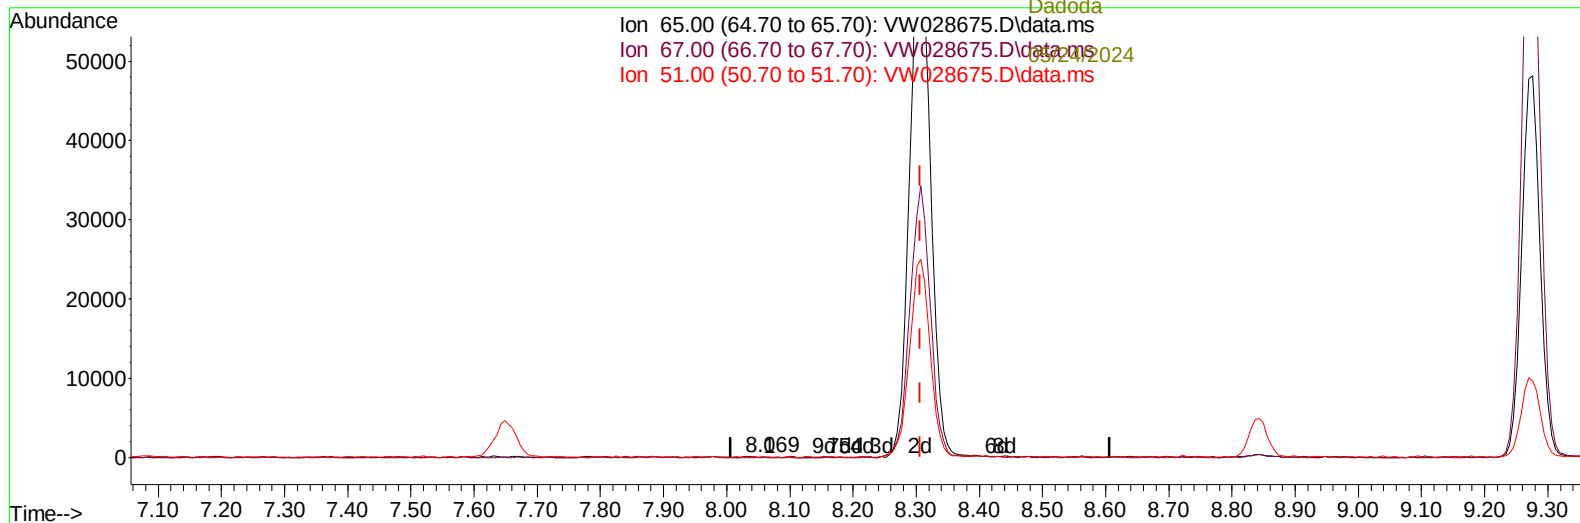

Scan 1014 (8.069 min): VW028675.D\data.ms

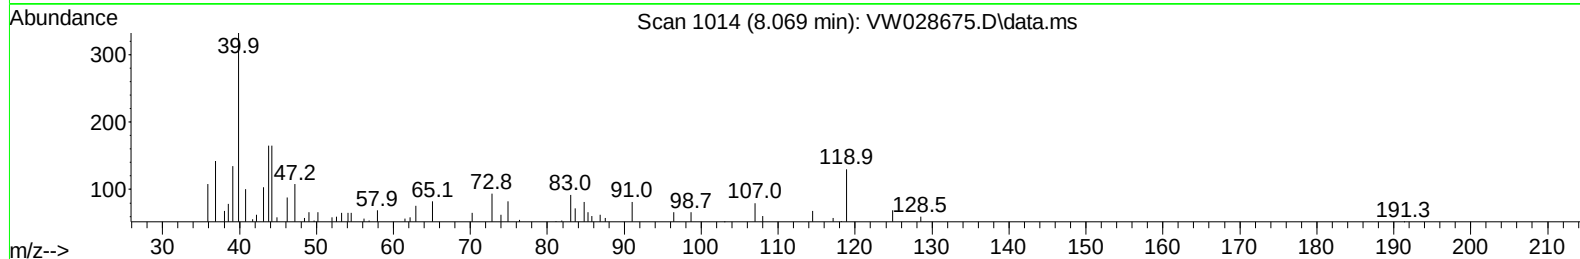

Scan 1053 (8.307 min): VW028673.D\data.ms (-1044) (-)

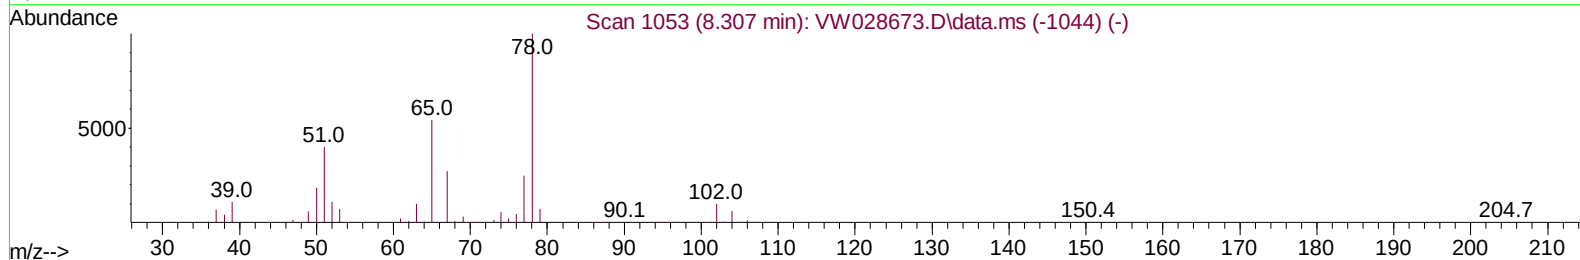

TIC: VW028675.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.069min (-0.238) 0.01 ug/L

response 52

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.60	57.69
51.00	101.70	88.46
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052224\
 Data File : VW028675.D
 Acq On : 22 May 2024 10:02
 Operator : SY/MD
 Sample : P2548-16
 Misc : 5.50g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH611




Manual IntegrationsAPPROVED

Quant Time: May 23 00:21:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 23 00:20:47 2024
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

05/23/2024
 Supervised By :Mahesh
 Dadoda

Ion 65.00 (64.70 to 65.70): VW028675.D\data.ms
 Ion 67.00 (66.70 to 67.70): VW028675.D\data.ms
 Ion 51.00 (50.70 to 51.70): VW028675.D\data.ms

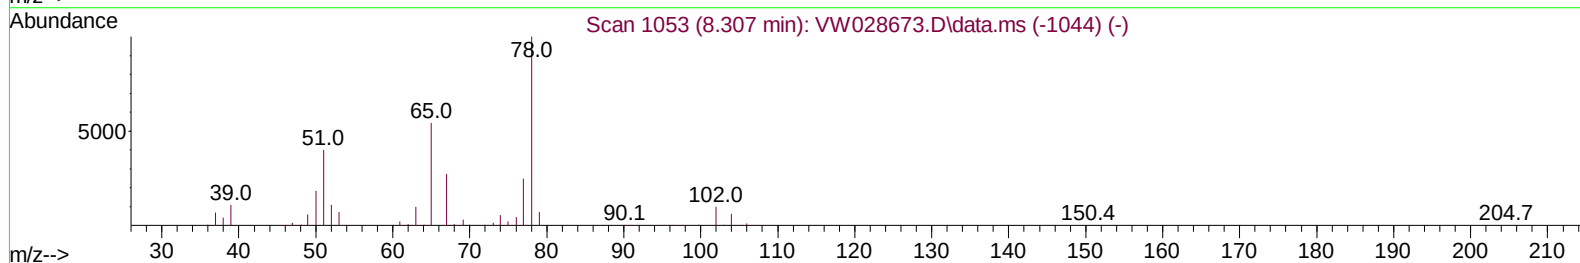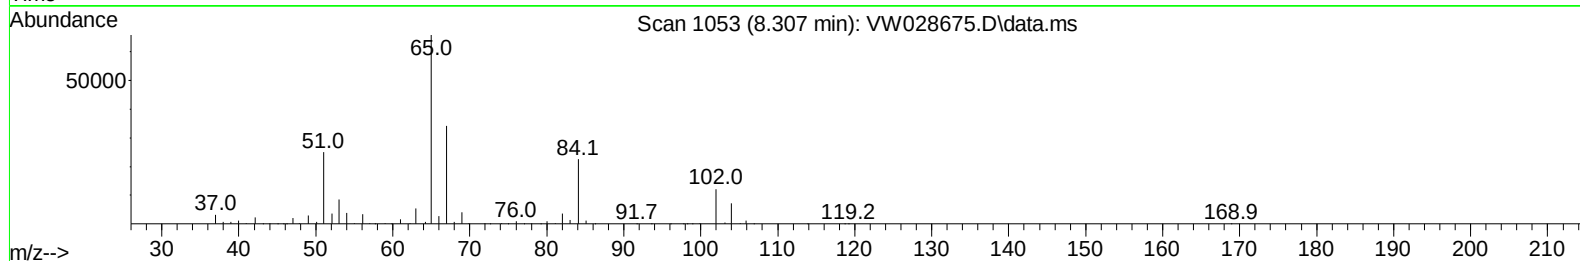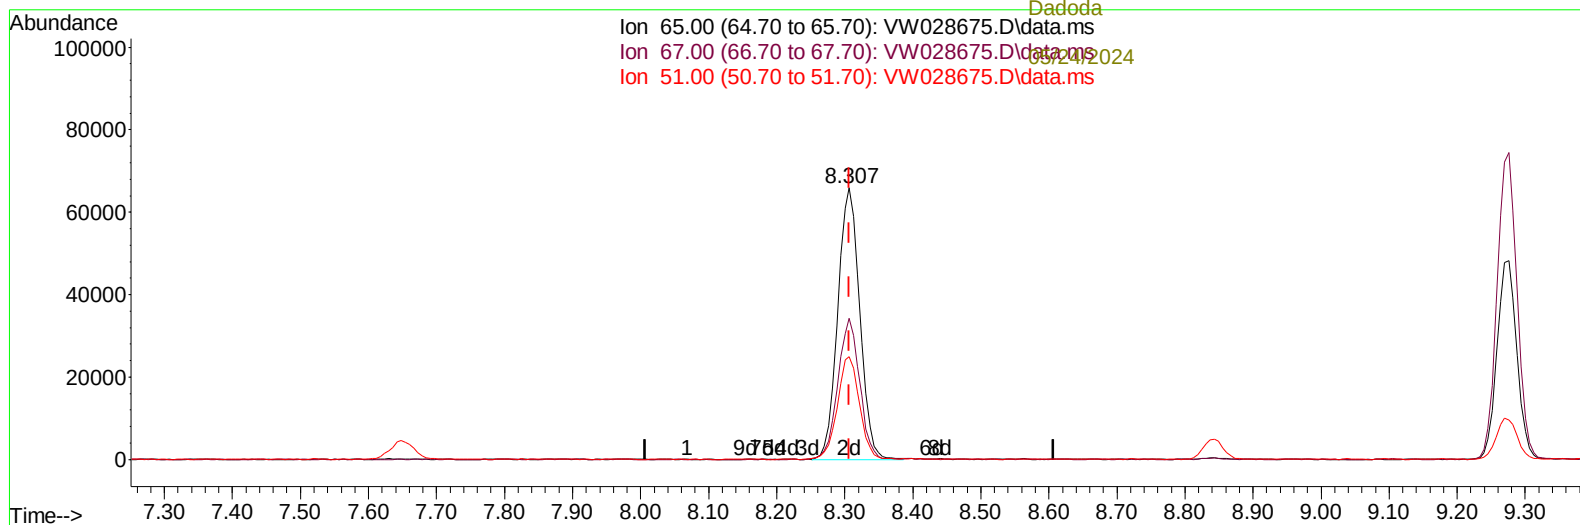

TIC: VW028675.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 19.06 ug/L m

response 147124

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.60	0.02#
51.00	101.70	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052224\
 Data File : VW028675.D
 Acq On : 22 May 2024 10:02
 Operator : SY/MD
 Sample : P2548-16
 Misc : 5.50g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH611

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

05/23/2024
 Supervised By :Mahesh
 Dadoda

Quant Time: May 23 00:21:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 23 00:20:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----05/24/2024						
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	431531	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	372930	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	149381	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	124240	15.161	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.640%	
7) Chloroethane-d5	2.899	69	107338	17.107	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	68.440%	
11) 1,1-Dichloroethene-d2	4.027	65	56095	16.385	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	65.520%	
21) 2-Butanone-d5	7.081	46	71178	33.294	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	66.580%	
24) Chloroform-d	7.648	84	251243m	18.633	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	74.520%	
26) 1,2-Dichloroethane-d4	8.307	65	147124m	19.058	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	76.240%	
32) Benzene-d6	8.276	84	481860	19.366	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	77.480%	
36) 1,2-Dichloropropane-d6	9.276	67	151171	20.191	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	80.760%	
41) Toluene-d8	10.318	98	411354	18.669	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	74.680%	
43) trans-1,3-Dichloroprop...	10.575	79	58456	19.408	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.640%	
47) 2-Hexanone-d5	10.922	63	49291	38.171	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	76.340%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	117952	18.787	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	75.160%	
66) 1,2-Dichlorobenzene-d4	13.848	152	117410	20.622	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	82.480%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052224\
Data File : VW028675.D
Acq On : 22 May 2024 10:02
Operator : SY/MD
Sample : P2548-16
Misc : 5.50g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH611

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

05/23/2024
Supervised By :Mahesh
Dadoda

05/24/2024

Quant Time: May 23 00:21:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 23 00:20:47 2024
Response via : Initial Calibration

