

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023237.D
 Acq On : 23 May 2022 09:49
 Operator : SY/VA
 Sample : VW0523SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK514

Quant Time: May 24 01:27:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	299685	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	291501	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	143381	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	130613	21.243	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.960%
7) Chloroethane-d5	2.885	69	84565	21.141	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.560%
11) 1,1-Dichloroethene-d2	4.135	63	366	0.046	ug/L	0.12
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.200%#
21) 2-Butanone-d5	7.080	46	49697	42.512	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.020%
24) Chloroform-d	7.647	84	214489	24.429	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.720%
26) 1,2-Dichloroethane-d4	8.403	65	222	0.046	ug/L	0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.200%#
32) Benzene-d6	8.275	84	424419	25.260	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.040%
36) 1,2-Dichloropropane-d6	9.275	67	122307	25.914	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.640%
41) Toluene-d8	10.323	98	404346	24.912	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.640%
43) trans-1,3-Dichloroprop...	10.579	79	51041	23.487	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.960%
47) 2-Hexanone-d5	10.927	63	38976	43.259	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.520%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	102753	23.358	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	132204	26.377	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.520%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	3922	0.609	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023237.D
Acq On : 23 May 2022 09:49
Operator : SY/VA
Sample : VW0523SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK514

Quant Time: May 24 01:27:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

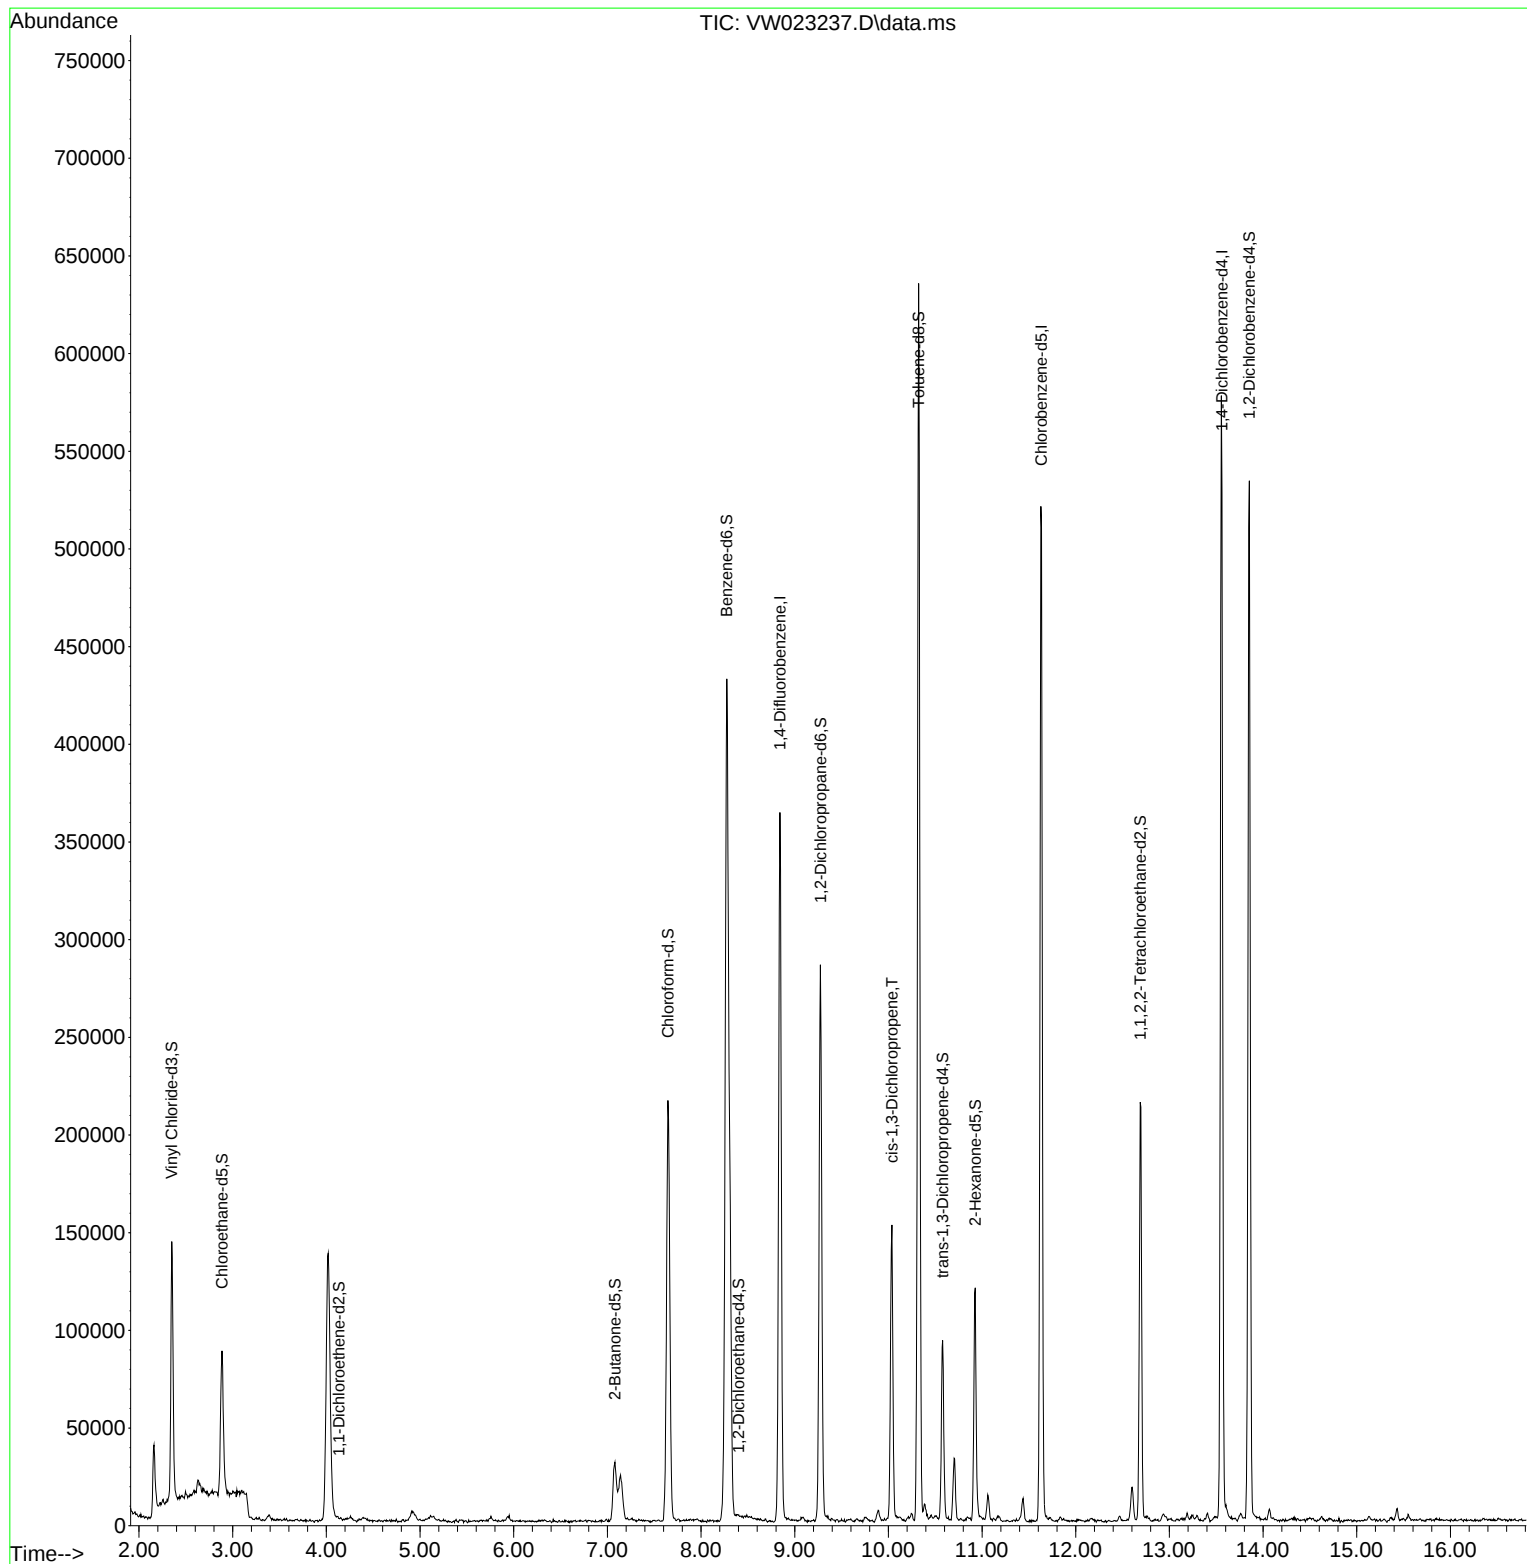

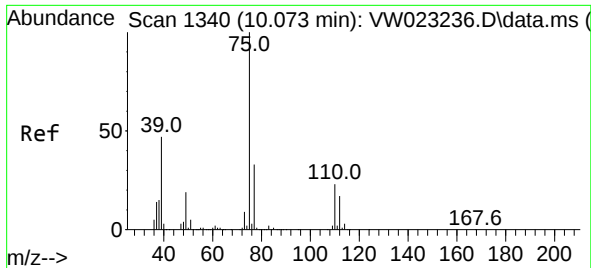

#39
 cis-1,3-Dichloropropene
 Concen: 0.609 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW023237.D
 Acq: 23 May 2022 09:49

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK514

Tgt Ion: 75 Resp: 3922
 Ion Ratio Lower Upper
 75 100
 77 49.6 22.1 41.1#

