

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023238.D
 Acq On : 23 May 2022 10:20
 Operator : SY/VA
 Sample : N2925-03RE
 Misc : 4.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY05

Quant Time: May 24 01:28:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	338060	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	328868	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	142458	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	120143	17.322	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.280%
7) Chloroethane-d5	2.885	69	86427	19.154	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.600%
11) 1,1-Dichloroethene-d2	4.019	63	129131	14.409	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.640%
21) 2-Butanone-d5	7.074	46	63973	48.512	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.020%
24) Chloroform-d	7.647	84	241269	24.360	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.440%
26) 1,2-Dichloroethane-d4	8.305	65	135778	24.995	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.000%
32) Benzene-d6	8.275	84	440914	23.260	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.040%
36) 1,2-Dichloropropane-d6	9.268	67	136632	25.660	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.640%
41) Toluene-d8	10.323	98	408597	22.314	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.240%
43) trans-1,3-Dichloroprop...	10.579	79	56471	23.033	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.120%
47) 2-Hexanone-d5	10.920	63	49535	48.732	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.460%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	119264	24.031	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	123605	24.821	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.280%
Target Compounds						
39) cis-1,3-Dichloropropene	10.036	75	4839	0.666	ug/L	Qvalue # 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023238.D
Acq On : 23 May 2022 10:20
Operator : SY/VA
Sample : N2925-03RE
Misc : 4.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY05

Quant Time: May 24 01:28:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

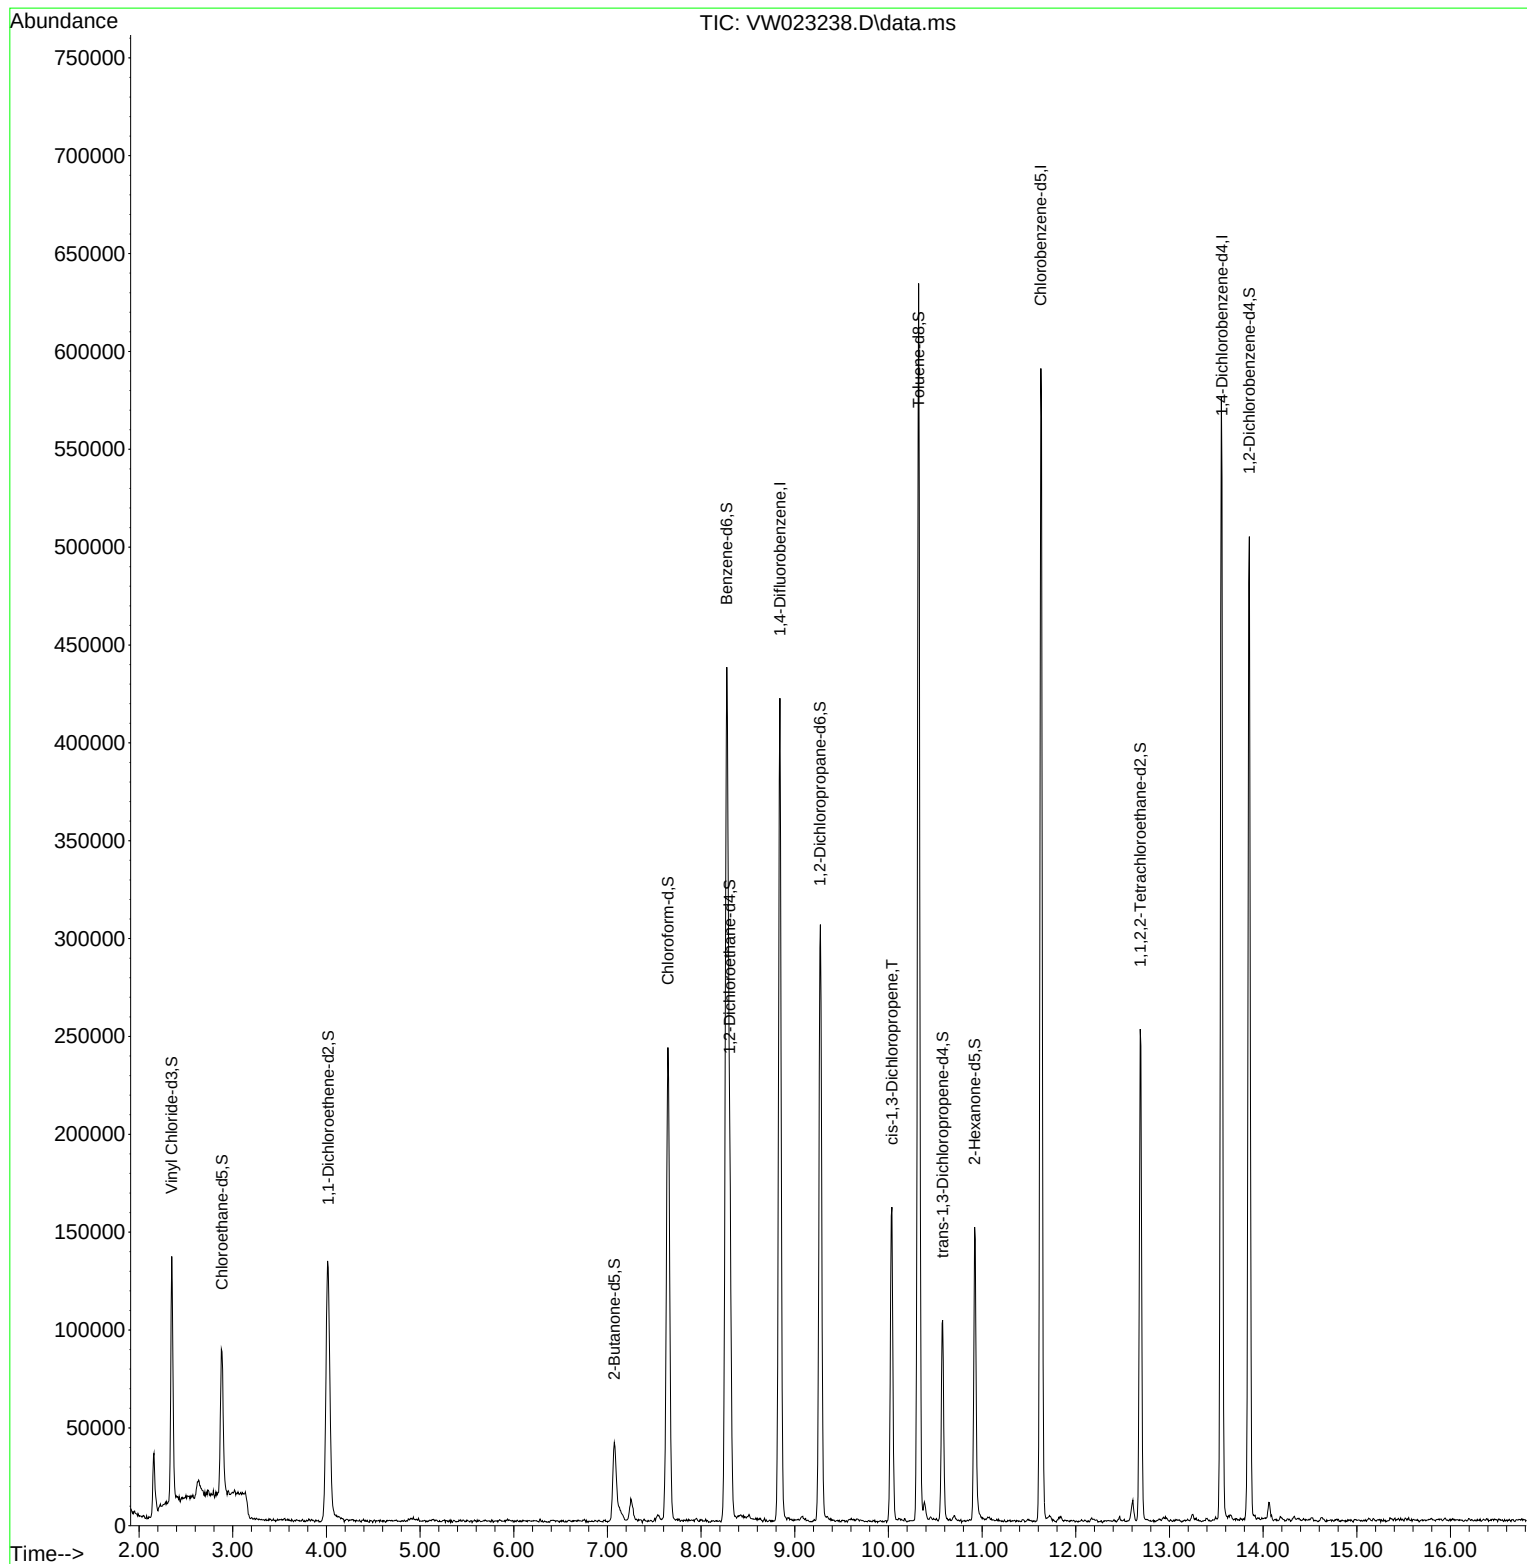

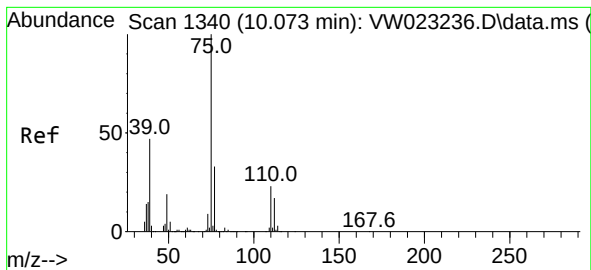

#39
 cis-1,3-Dichloropropene
 Concen: 0.666 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023238.D
 Acq: 23 May 2022 10:20

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY05

Tgt Ion: 75 Resp: 4839
 Ion Ratio Lower Upper
 75 100
 77 56.5 22.1 41.1#

