

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023243.D
 Acq On : 23 May 2022 12:21
 Operator : SY/VA
 Sample : N2926-08
 Misc : 4.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY17

Quant Time: May 24 01:29:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	362075	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	362898	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	173025	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	134803	18.147	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.600%
7) Chloroethane-d5	2.885	69	98086	20.296	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.200%
11) 1,1-Dichloroethene-d2	4.013	63	139326	14.515	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.080%
21) 2-Butanone-d5	7.080	46	77678	54.997	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.000%
24) Chloroform-d	7.647	84	260174	24.526	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.120%
26) 1,2-Dichloroethane-d4	8.305	65	153730	26.423	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.680%
32) Benzene-d6	8.275	84	479288	22.914	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.640%
36) 1,2-Dichloropropane-d6	9.274	67	149738	25.484	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.920%
41) Toluene-d8	10.323	98	458525	22.692	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.760%
43) trans-1,3-Dichloroprop...	10.579	79	63634	23.521	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.080%
47) 2-Hexanone-d5	10.927	63	62073	55.340	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.680%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	144422	26.371	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.480%
66) 1,2-Dichlorobenzene-d4	13.853	152	161046	26.626	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.520%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	5695	0.710	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023243.D
Acq On : 23 May 2022 12:21
Operator : SY/VA
Sample : N2926-08
Misc : 4.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY17

Quant Time: May 24 01:29:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

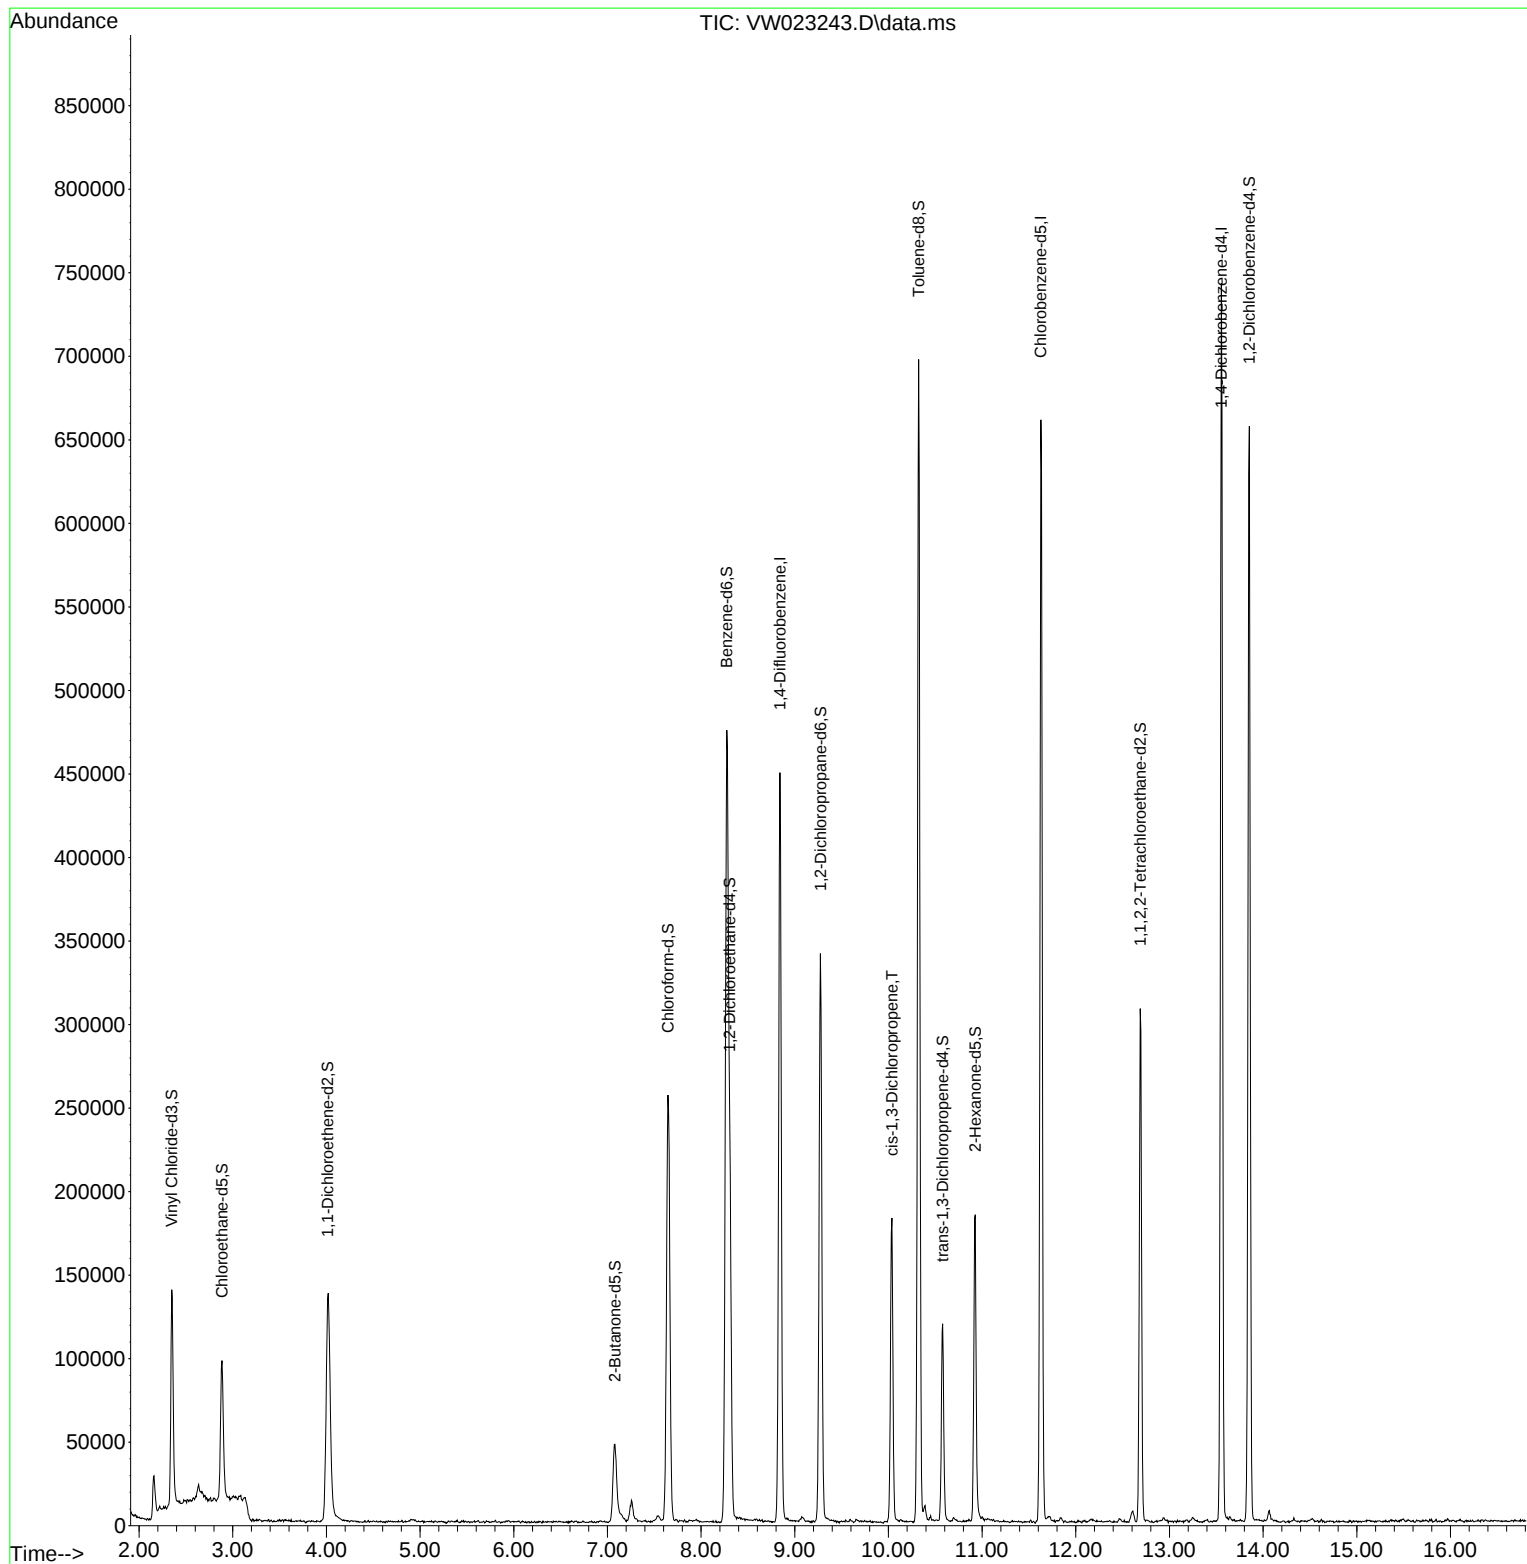

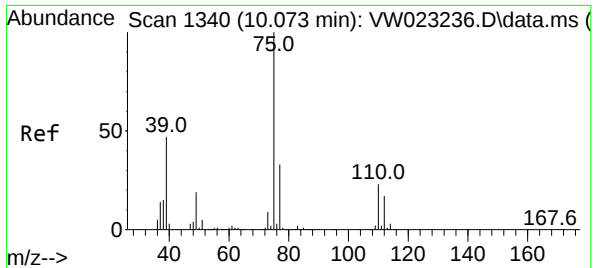

#39

cis-1,3-Dichloropropene

Concen: 0.710 ug/L

RT: 10.036 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW023243.D


Acq: 23 May 2022 12:21

Instrument :

MSVOA_W

ClientSampleId :

EXY17

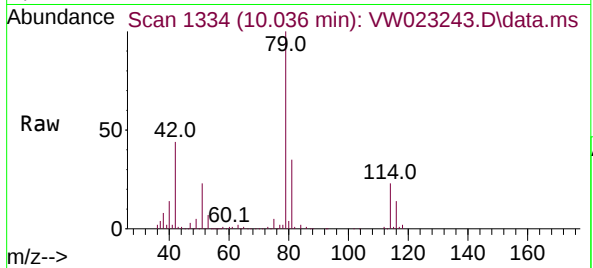

Tgt Ion: 75 Resp: 5695

Ion Ratio Lower Upper

75 100

77 40.3 22.1 41.1

