

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023244.D
 Acq On : 23 May 2022 12:45
 Operator : SY/VA
 Sample : N2926-09
 Misc : 4.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY18

Quant Time: May 24 01:29:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	358054	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	343982	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	156457	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	133202	18.133	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.520%
7) Chloroethane-d5	2.879	69	94031	19.675	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.720%
11) 1,1-Dichloroethene-d2	4.013	63	130246	13.722	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.880%
21) 2-Butanone-d5	7.080	46	68431	48.994	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.980%
24) Chloroform-d	7.647	84	245680	23.420	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.680%
26) 1,2-Dichloroethane-d4	8.305	65	144293	25.079	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.320%
32) Benzene-d6	8.275	84	450910	22.742	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.960%
36) 1,2-Dichloropropane-d6	9.275	67	142284	25.547	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.200%
41) Toluene-d8	10.323	98	419498	21.903	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.600%
43) trans-1,3-Dichloroprop...	10.579	79	57752	22.521	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.080%
47) 2-Hexanone-d5	10.921	63	53149	49.990	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.980%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	131302	25.294	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	133262	24.366	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.480%
Target Compounds						
39) cis-1,3-Dichloropropene	10.037	75	5006	0.658	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023244.D
Acq On : 23 May 2022 12:45
Operator : SY/VA
Sample : N2926-09
Misc : 4.80g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY18

Quant Time: May 24 01:29:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

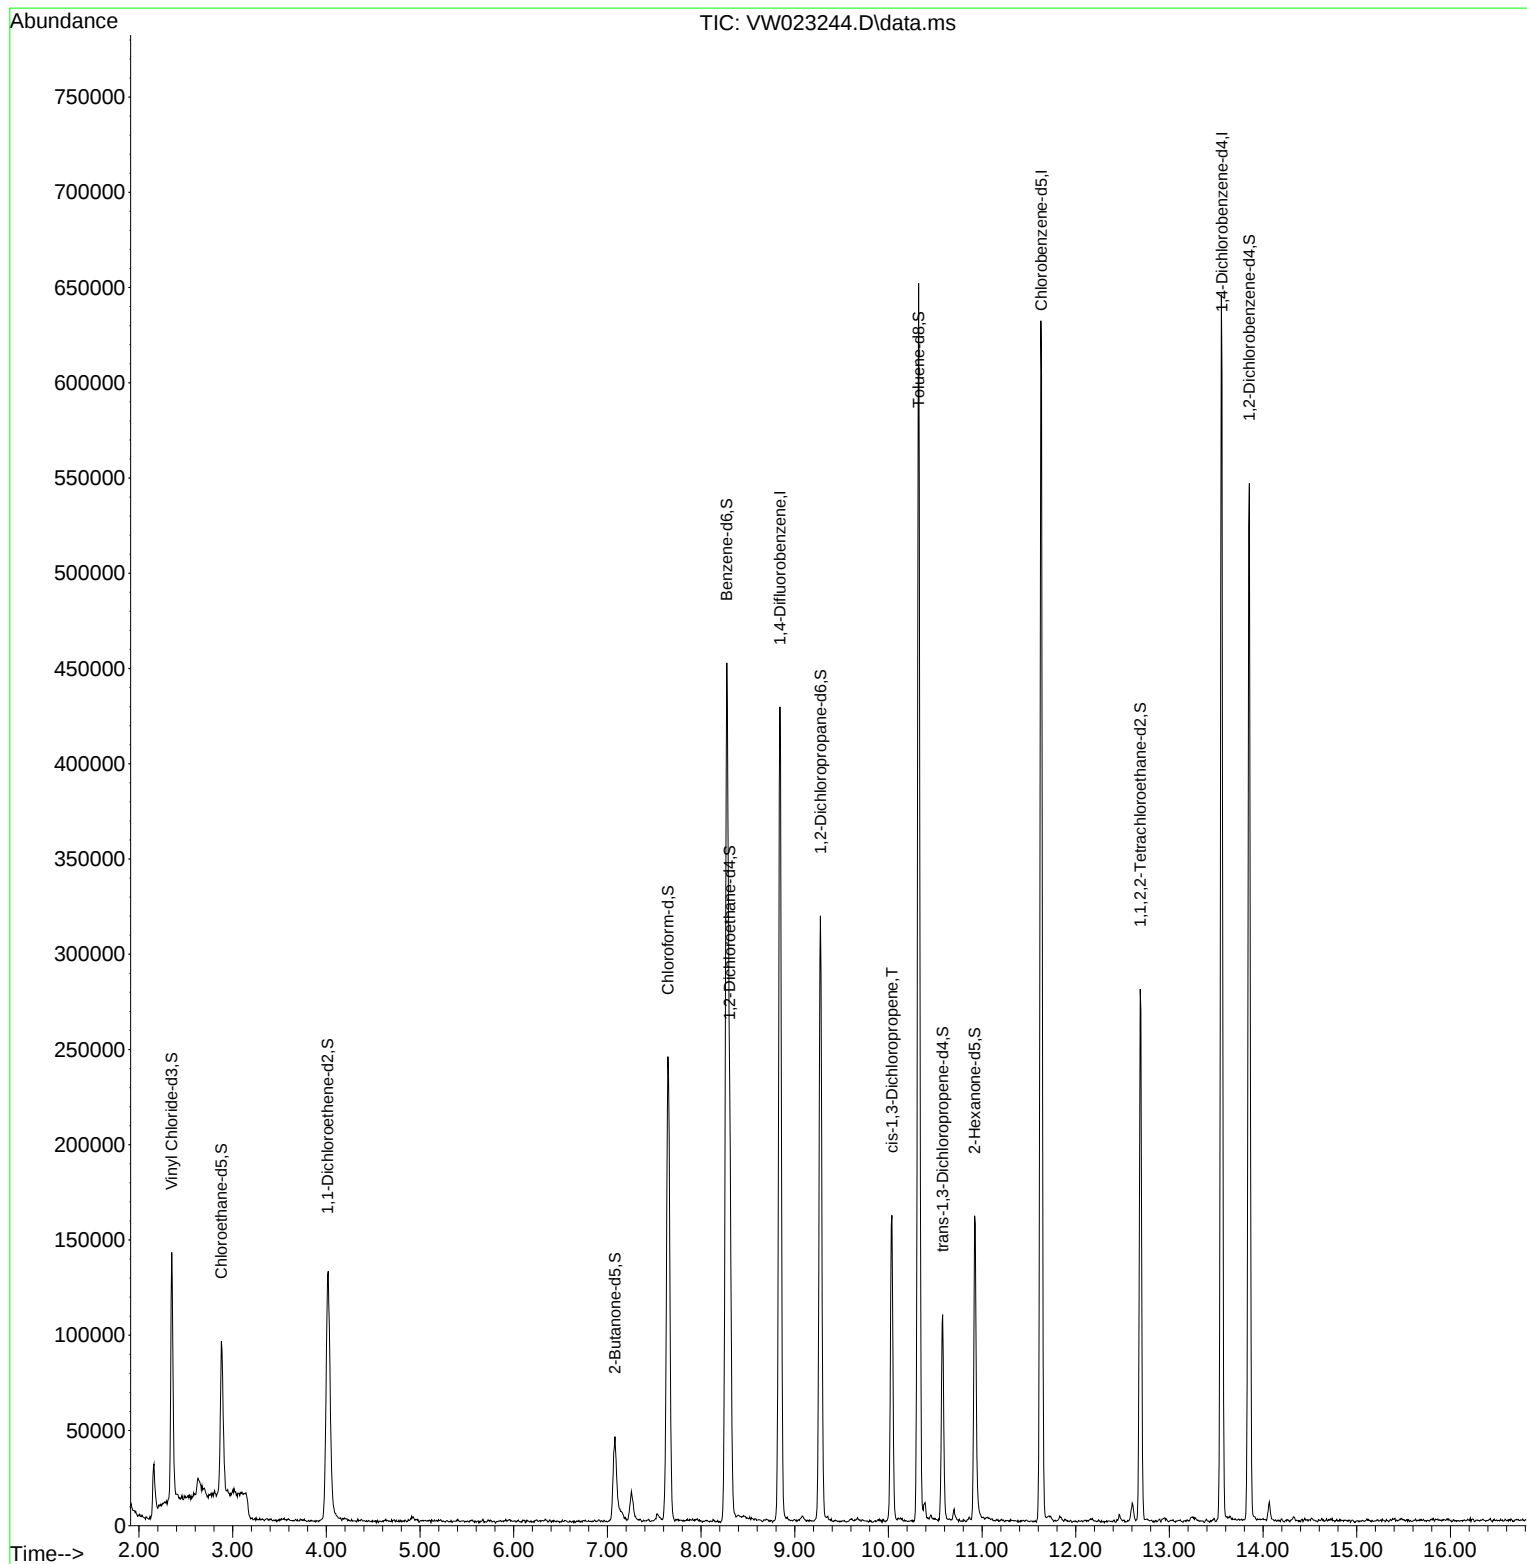

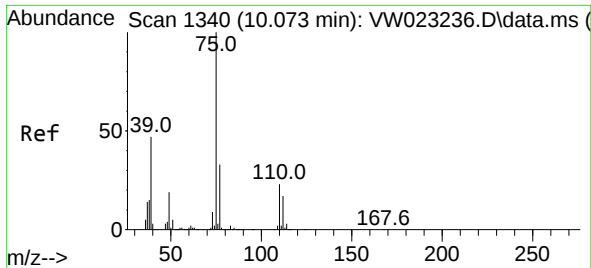

#39
 cis-1,3-Dichloropropene
 Concen: 0.658 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW023244.D
 Acq: 23 May 2022 12:45

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY18

Tgt Ion: 75 Resp: 5006
 Ion Ratio Lower Upper
 75 100
 77 33.0 22.1 41.1

