

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023245.D
 Acq On : 23 May 2022 13:09
 Operator : SY/VA
 Sample : N2926-10
 Misc : 3.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY19

Quant Time: May 24 01:29:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	314996	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	246092	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	67502	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	134011	20.736	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.960%
7) Chloroethane-d5	2.885	69	96029	22.840	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.360%
11) 1,1-Dichloroethene-d2	4.019	63	129075	15.457	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.840%
21) 2-Butanone-d5	7.079	46	43645	35.520	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.040%
24) Chloroform-d	7.646	84	234708	25.433	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.720%
26) 1,2-Dichloroethane-d4	8.305	65	131922	26.064	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.240%
32) Benzene-d6	8.274	84	422296	29.771	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	119.080%
36) 1,2-Dichloropropane-d6	9.274	67	130922	32.858	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	131.440%#
41) Toluene-d8	10.323	98	362100	26.426	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.720%
43) trans-1,3-Dichloroprop...	10.579	79	39297	21.420	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.680%
47) 2-Hexanone-d5	10.926	63	31234	41.063	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.120%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	91780	24.713	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	62726	26.583	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.320%
Target Compounds					Qvalue	
48) 2-Hexanone	10.945	43	5571	3.771	ug/L #	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023245.D
Acq On : 23 May 2022 13:09
Operator : SY/VA
Sample : N2926-10
Misc : 3.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY19


Quant Time: May 24 01:29:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

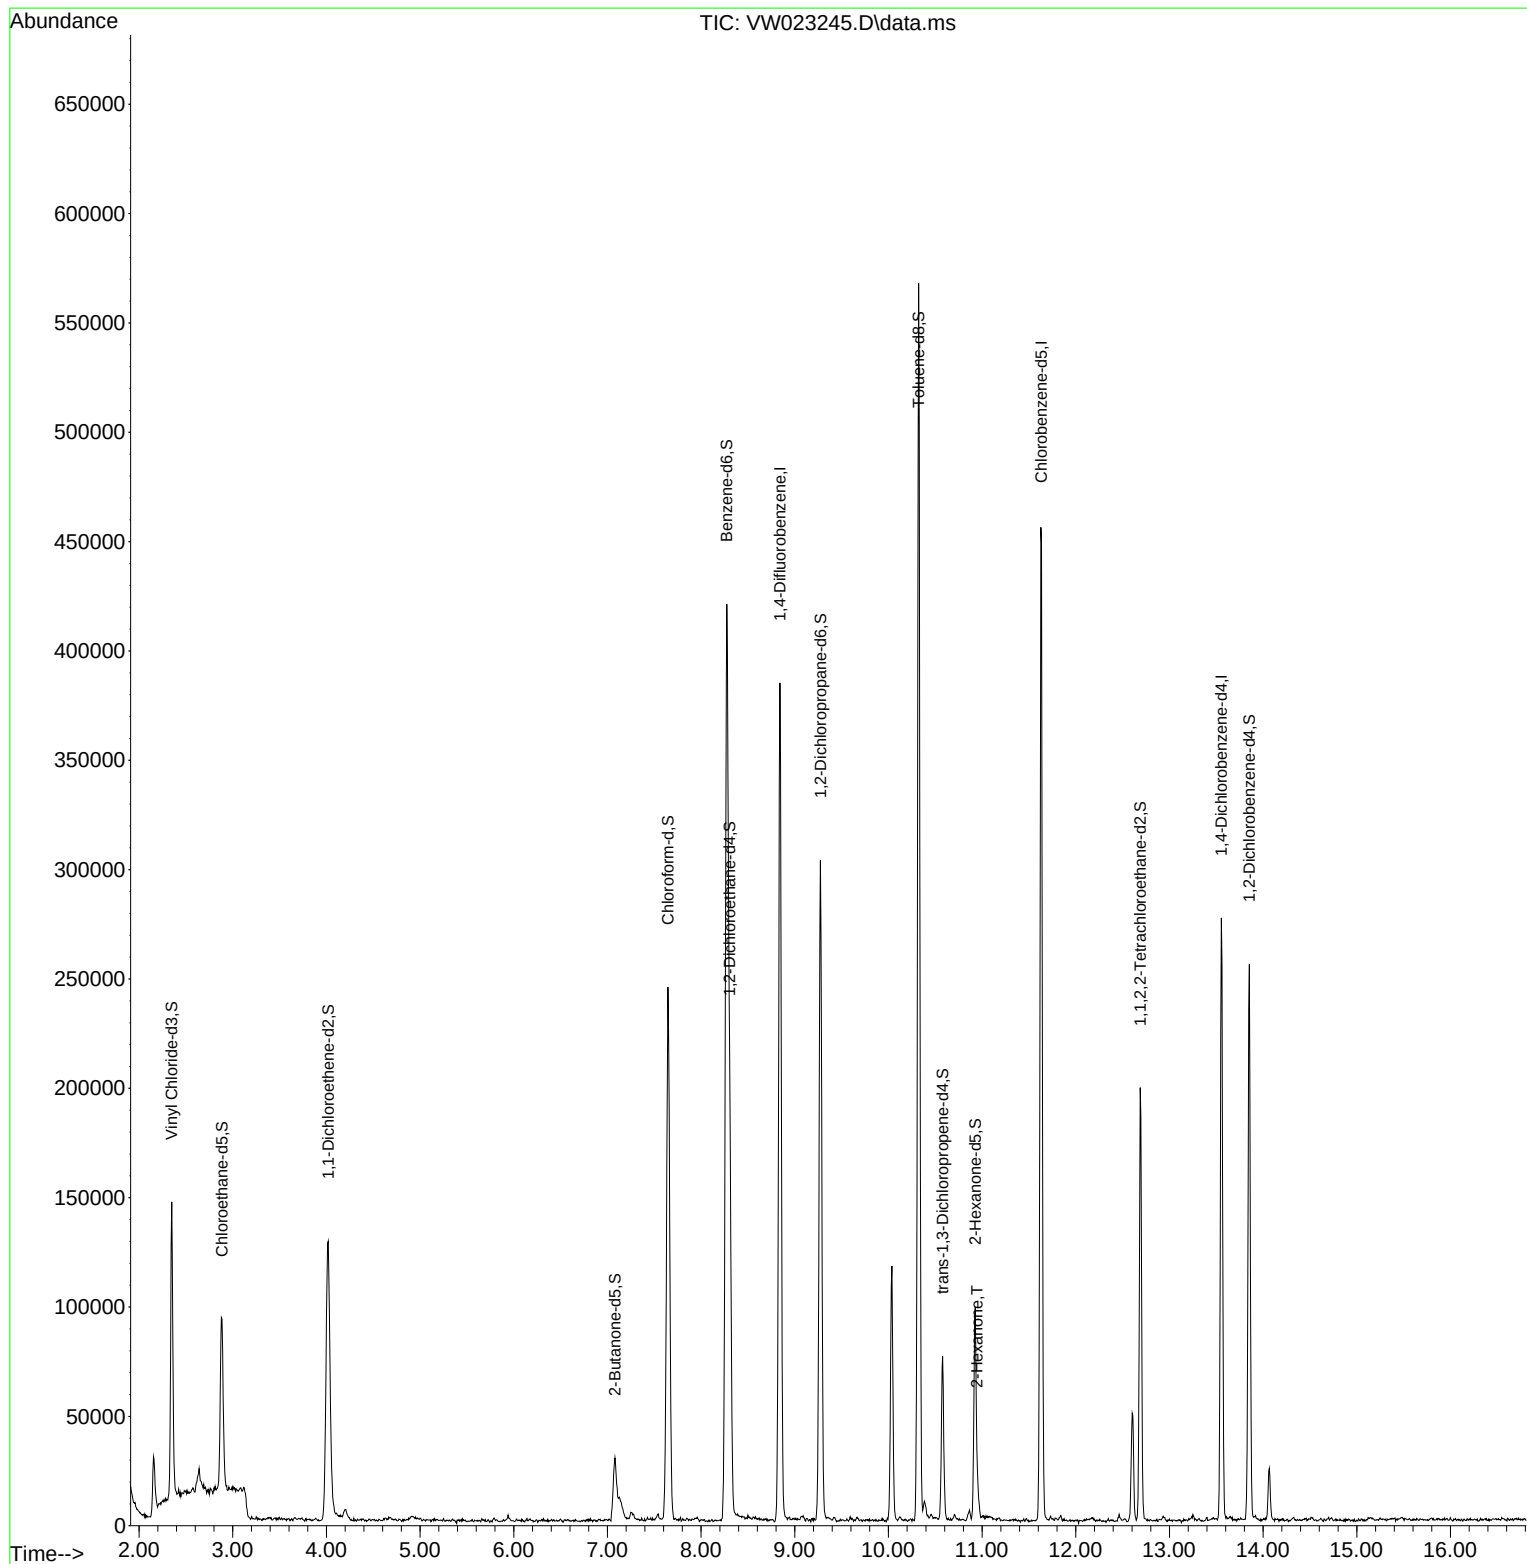

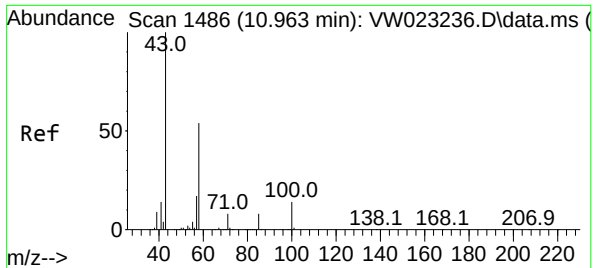

#48
 2-Hexanone
 Concen: 3.771 ug/L
 RT: 10.945 min Scan# 1483
 Delta R.T. -0.018 min
 Lab File: VW023245.D
 Acq: 23 May 2022 13:09

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY19

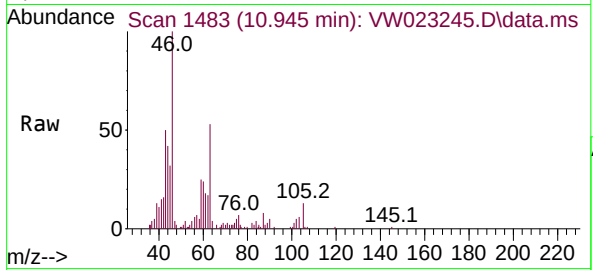

Tgt Ion: 43	Resp:	5571
Ion	Ratio	Lower Upper
43	100	
58	9.5	45.9 68.9#
57	0.8	16.2 24.2#
100	0.8	10.7 16.1#

