

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023247.D
 Acq On : 23 May 2022 13:58
 Operator : SY/VA
 Sample : N2926-12
 Misc : 4.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY21

Quant Time: May 24 01:29:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	350284	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	344809	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	155883	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	122116	16.992	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.960%
7) Chloroethane-d5	2.879	69	82147	17.570	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.280%
11) 1,1-Dichloroethene-d2	4.013	63	117691	12.674	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.680%
21) 2-Butanone-d5	7.080	46	58255	42.634	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.260%
24) Chloroform-d	7.647	84	225043	21.929	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.720%
26) 1,2-Dichloroethane-d4	8.305	65	130282	23.147	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.600%
32) Benzene-d6	8.275	84	420262	21.146	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.600%
36) 1,2-Dichloropropane-d6	9.268	67	128644	23.043	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.160%
41) Toluene-d8	10.323	98	384932	20.050	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.200%
43) trans-1,3-Dichloroprop...	10.579	79	50376	19.597	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.400%
47) 2-Hexanone-d5	10.920	63	44114	41.392	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.780%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	118514	22.776	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	124265	22.804	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.200%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4600	0.604	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023247.D
Acq On : 23 May 2022 13:58
Operator : SY/VA
Sample : N2926-12
Misc : 4.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY21

Quant Time: May 24 01:29:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

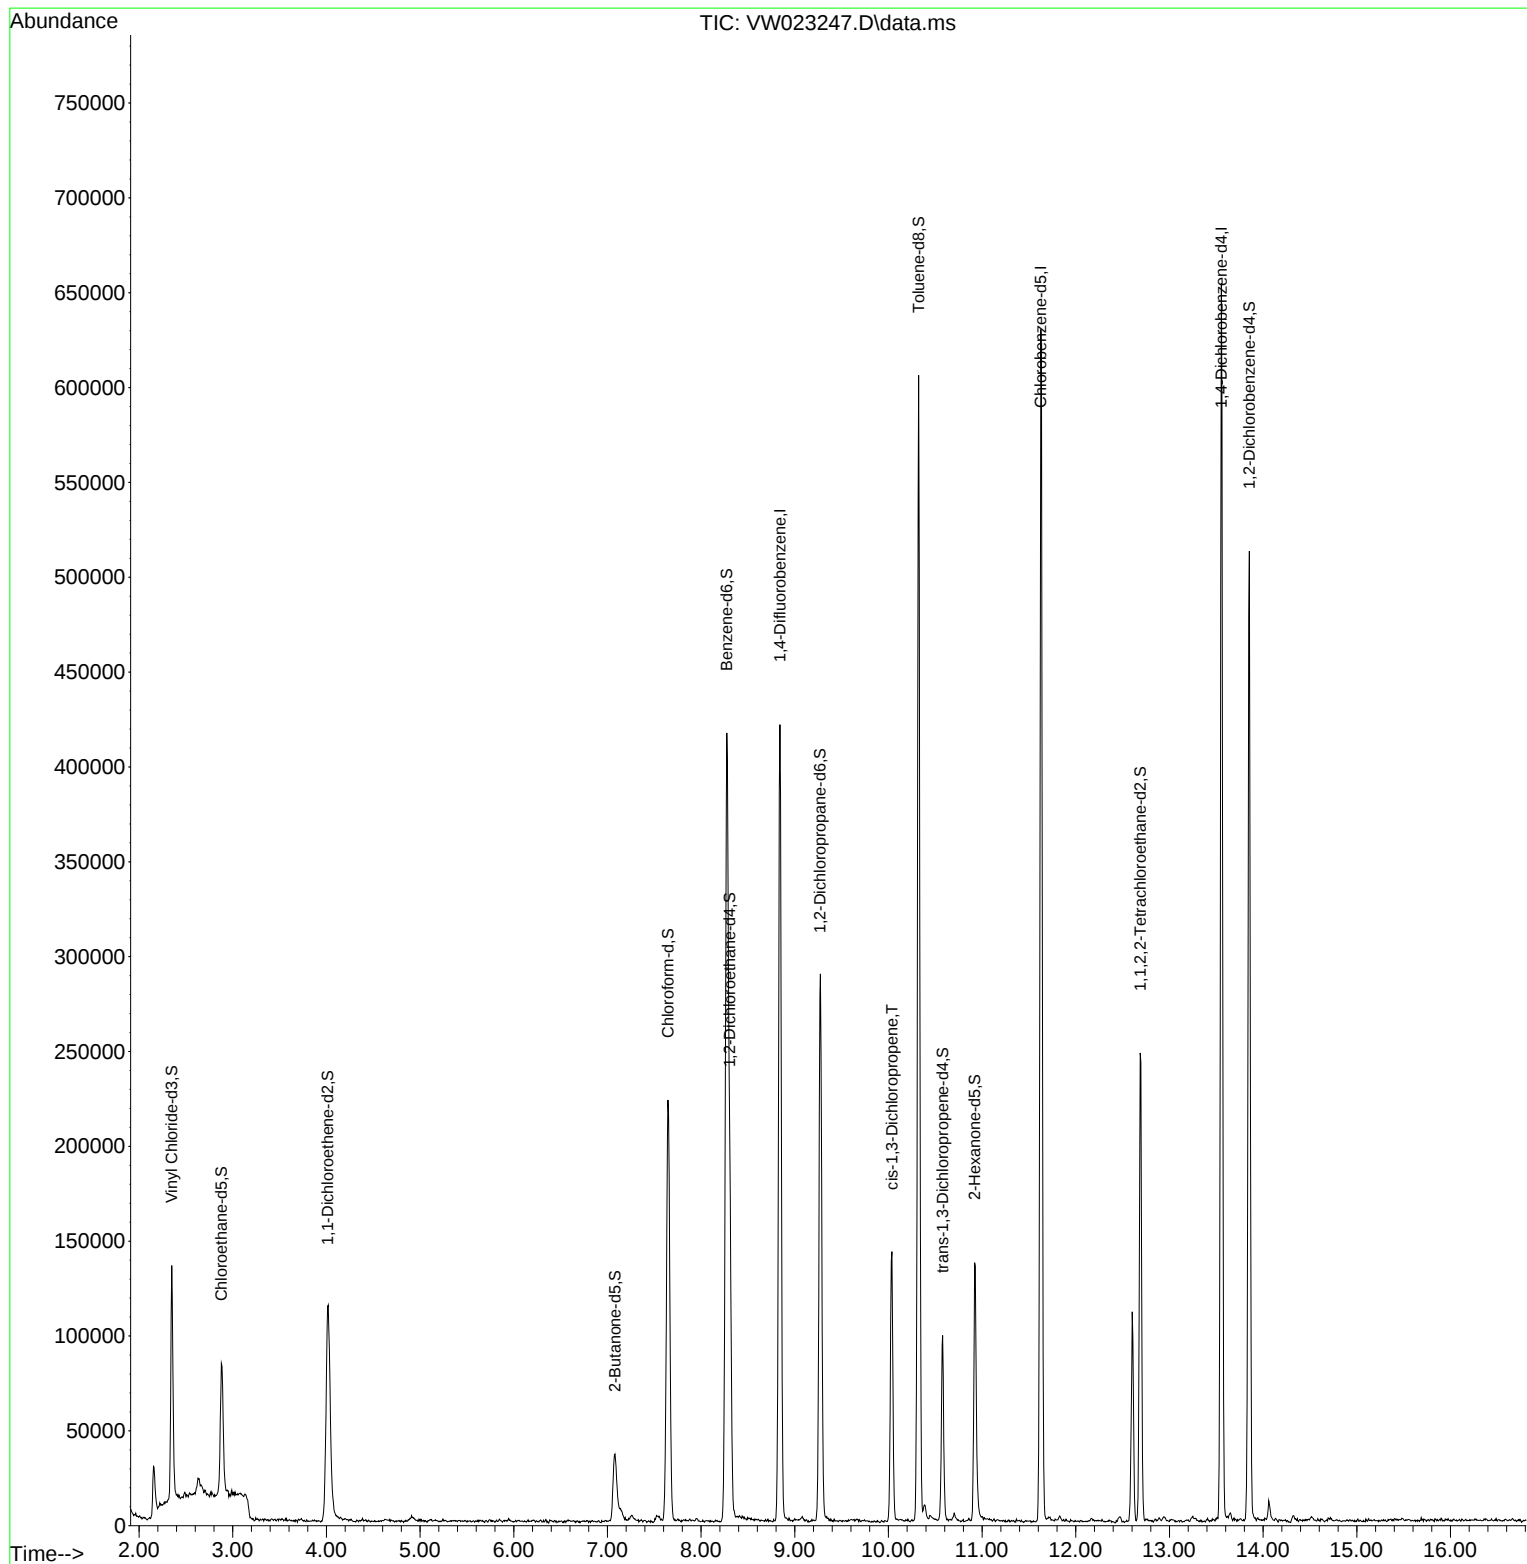

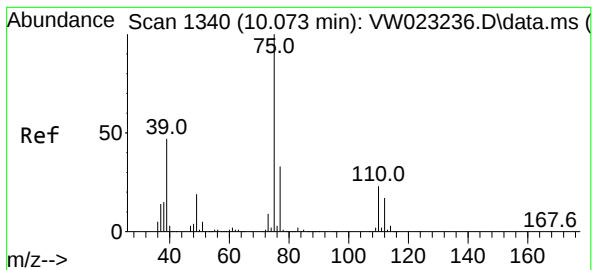

#39
 cis-1,3-Dichloropropene
 Concen: 0.604 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023247.D
 Acq: 23 May 2022 13:58

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY21

Tgt Ion: 75 Resp: 4600
 Ion Ratio Lower Upper
 75 100
 77 40.7 22.1 41.1

