

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023254.D
 Acq On : 23 May 2022 16:47
 Operator : SY/VA
 Sample : N2925-02RE
 Misc : 4.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY04

Quant Time: May 24 01:31:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	329656	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	326573	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	149620	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	138354	20.456	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.840%
7) Chloroethane-d5	2.879	69	96193	21.861	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.440%
11) 1,1-Dichloroethene-d2	4.202	63	236	0.027	ug/L	0.18
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.120%#
21) 2-Butanone-d5	7.080	46	68086	52.947	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.900%
24) Chloroform-d	7.647	84	244611	25.327	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.320%
26) 1,2-Dichloroethane-d4	8.384	65	259	0.049	ug/L	0.08
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.200%#
32) Benzene-d6	8.275	84	446928	23.743	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.960%
36) 1,2-Dichloropropane-d6	9.275	67	138541	26.201	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.800%
41) Toluene-d8	10.323	98	409133	22.500	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.000%
43) trans-1,3-Dichloroprop...	10.579	79	55583	22.830	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.320%
47) 2-Hexanone-d5	10.921	63	55940	55.420	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.840%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	129832	26.344	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	132525	25.338	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.360%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	4804	0.665	ug/L	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023254.D
Acq On : 23 May 2022 16:47
Operator : SY/VA
Sample : N2925-02RE
Misc : 4.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY04

Quant Time: May 24 01:31:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

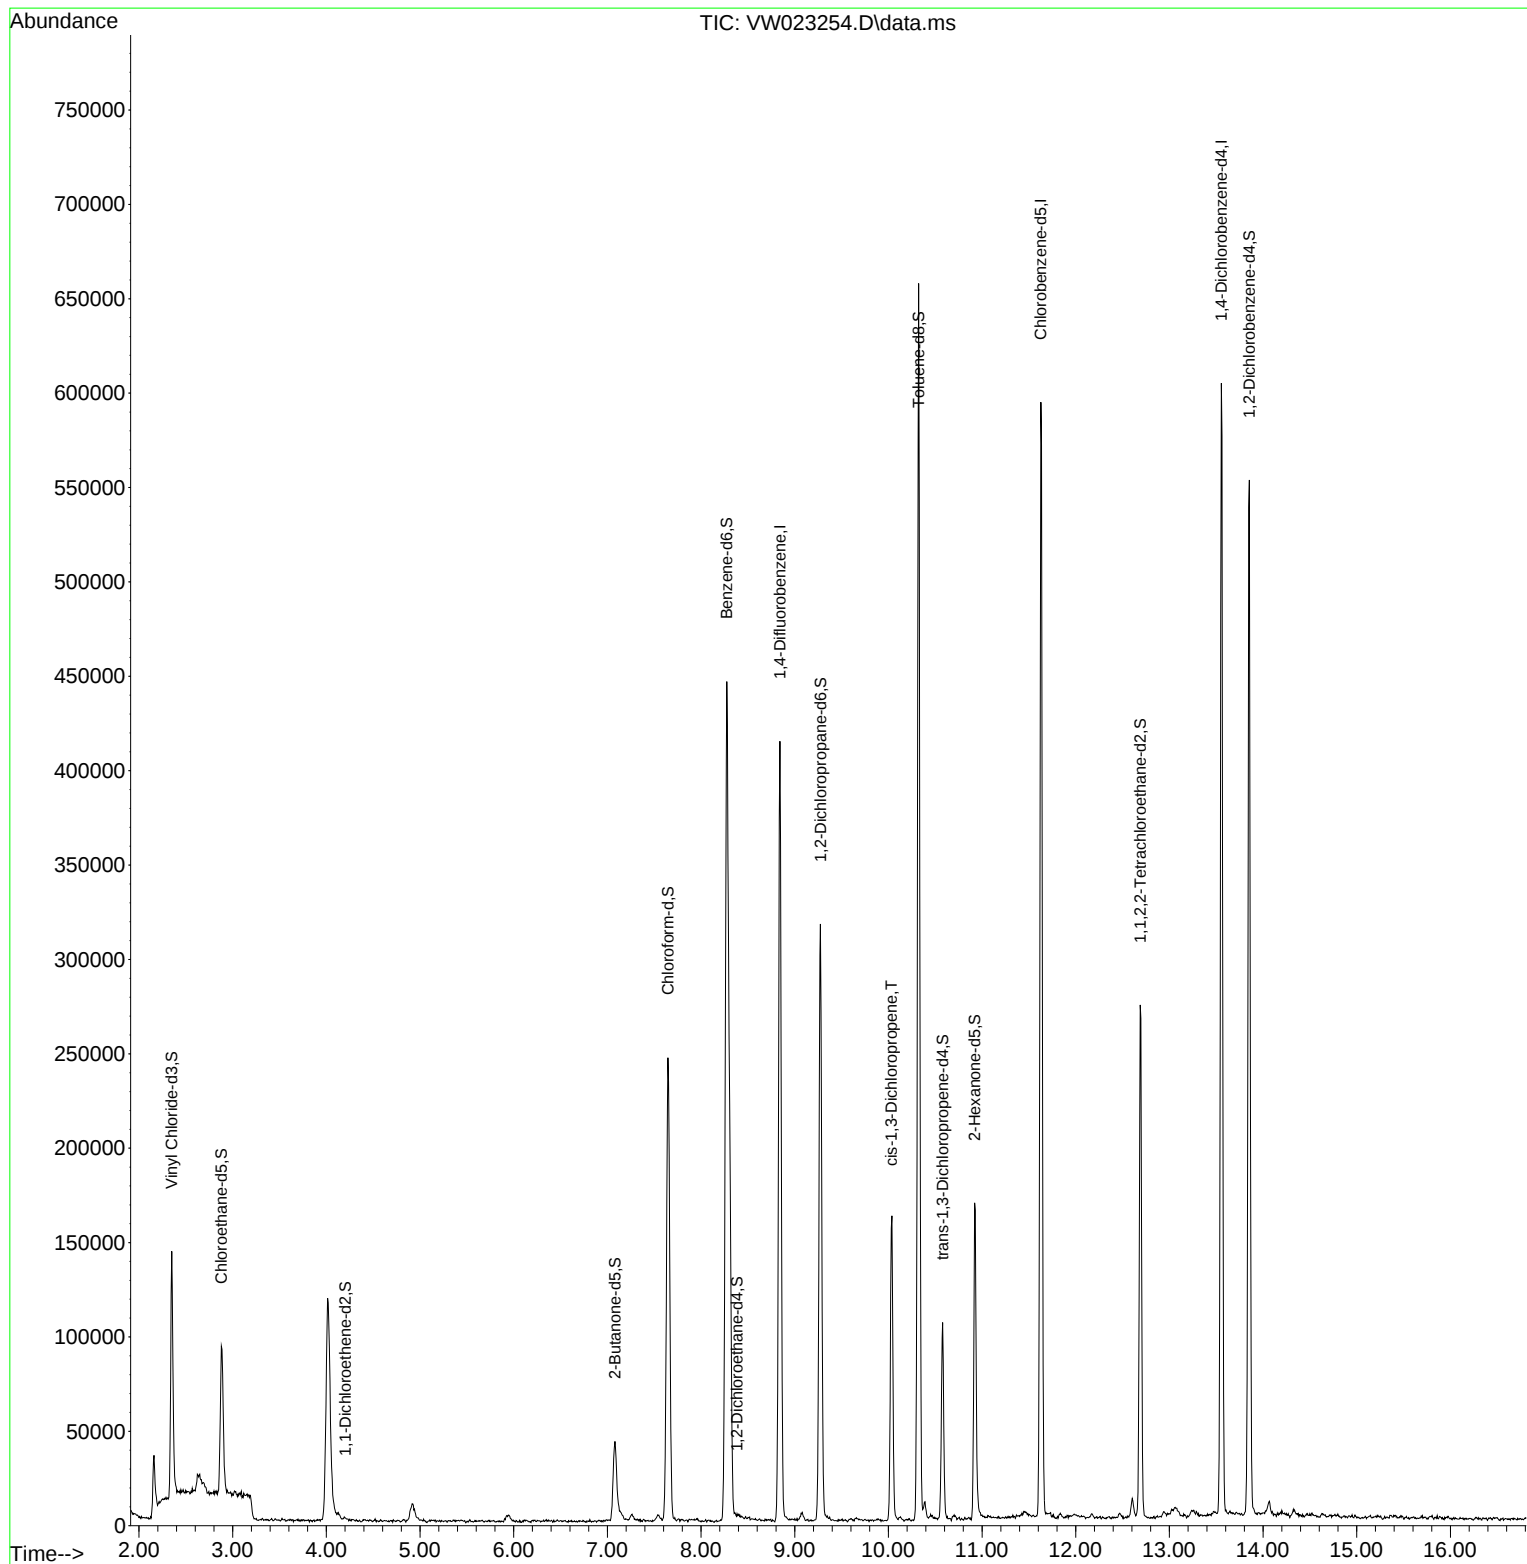

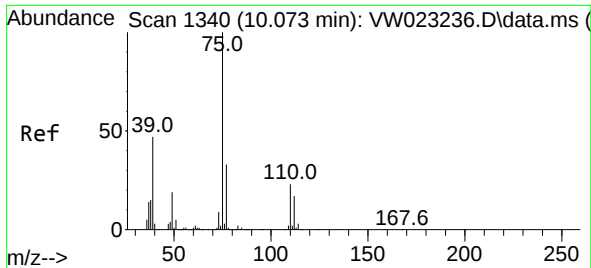

#39
 cis-1,3-Dichloropropene
 Concen: 0.665 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW023254.D
 Acq: 23 May 2022 16:47

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY04

Tgt Ion: 75 Resp: 4804
 Ion Ratio Lower Upper
 75 100
 77 42.6 22.1 41.1#

