




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023239.D
 Acq On : 23 May 2022 10:44
 Operator : SY/VA
 Sample : N2925-05
 Misc : 4.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY07

Manual IntegrationsAPPROVED

Quant Time: May 24 01:28:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/24/2022
 Supervised By :Mahesh Dadoda 05/25/2022

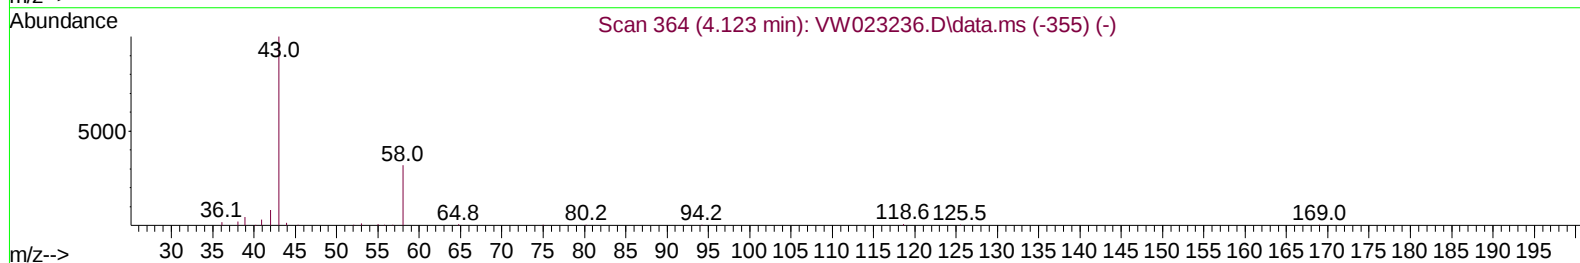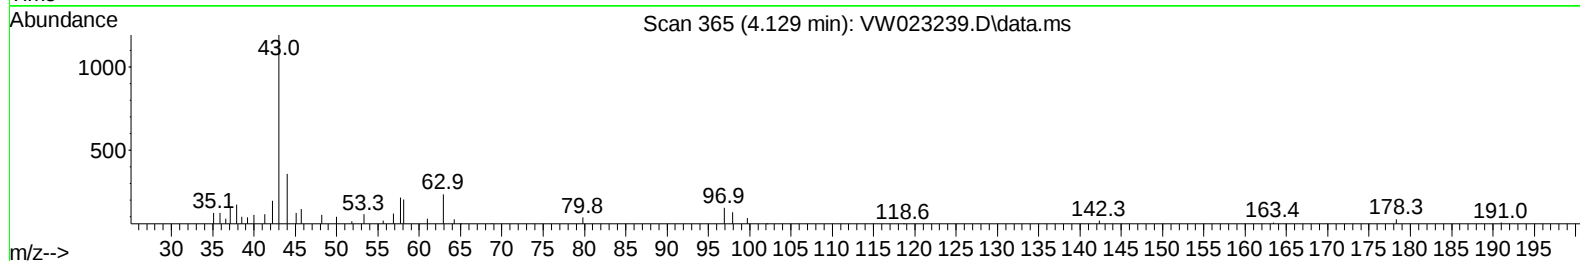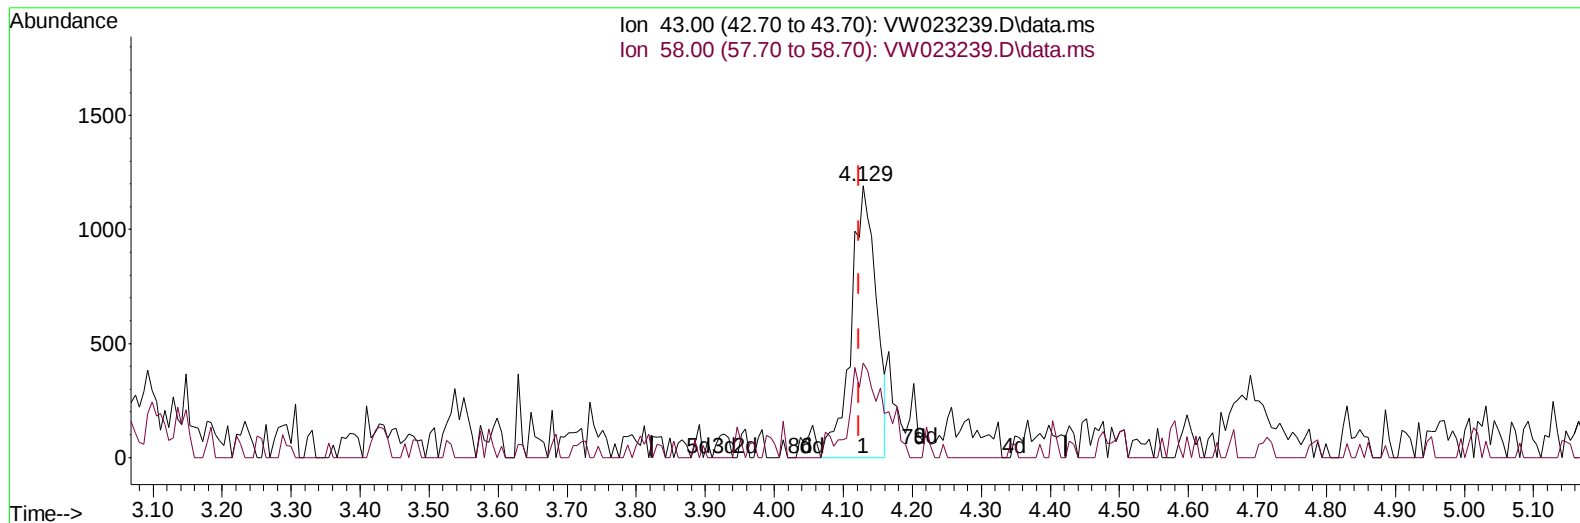

TIC: VW023239.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 3.34 ug/L

response 2995

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	16.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023239.D
 Acq On : 23 May 2022 10:44
 Operator : SY/VA
 Sample : N2925-05
 Misc : 4.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY07

Manual IntegrationsAPPROVED

Quant Time: May 24 01:28:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/24/2022
 Supervised By :Mahesh Dadoda 05/25/2022

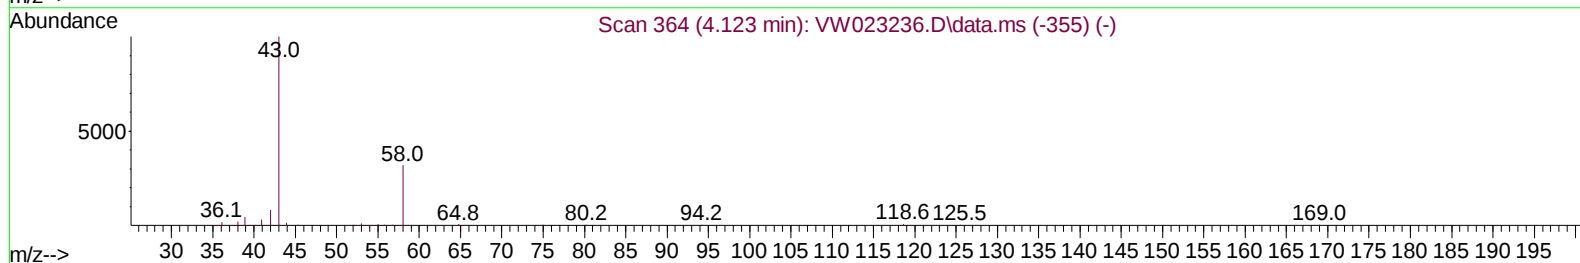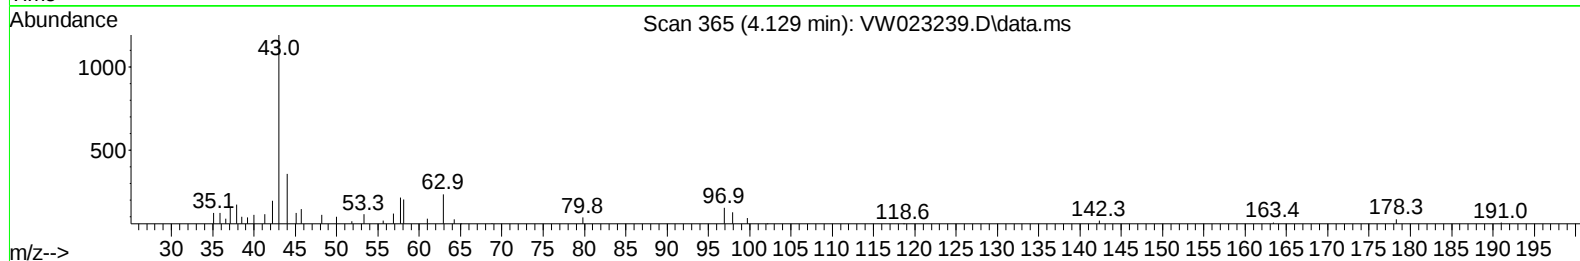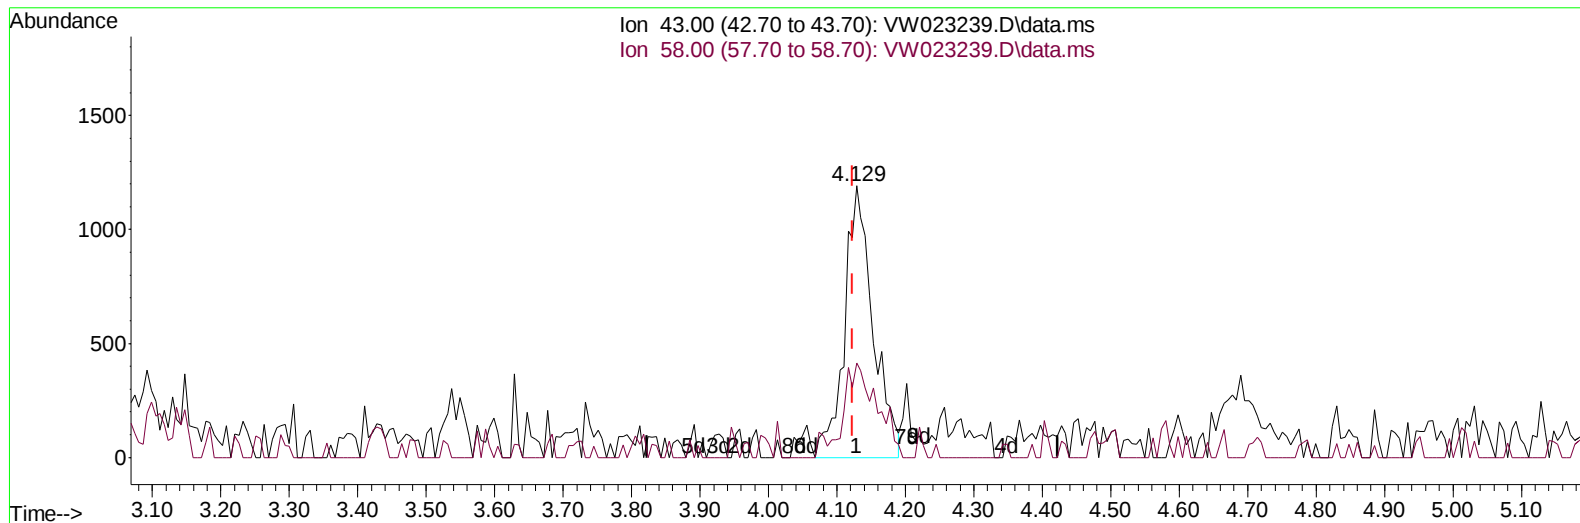

TIC: VW023239.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 3.82 ug/L m

response 3426

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	14.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023239.D
 Acq On : 23 May 2022 10:44
 Operator : SY/VA
 Sample : N2925-05
 Misc : 4.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY07

Manual IntegrationsAPPROVED

Quant Time: May 24 01:28:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/24/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	307336	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	295044	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	129118	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	113380	17.981	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.920%	
7) Chloroethane-d5	2.885	69	79848	19.465	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.840%	
11) 1,1-Dichloroethene-d2	4.013	63	120876	14.836	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	59.360%	
21) 2-Butanone-d5	7.074	46	59601	49.714	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	99.420%	
24) Chloroform-d	7.653	84	217073	24.108	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.440%	
26) 1,2-Dichloroethane-d4	8.305	65	125255	25.363	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	101.440%	
32) Benzene-d6	8.275	84	402806	23.686	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	94.760%	
36) 1,2-Dichloropropane-d6	9.274	67	121953	25.529	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	102.120%	
41) Toluene-d8	10.323	98	377490	22.978	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	91.920%	
43) trans-1,3-Dichloroprop...	10.579	79	51584	23.452	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	93.800%	
47) 2-Hexanone-d5	10.920	63	46397	50.878	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	101.760%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	112654	25.301	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	13.853	152	120519	26.702	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	106.800%	
Target Compounds						
13) Acetone	4.129	43	3426m	3.817	ug/L	
33) Benzene	8.329	78	10384	0.597	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023239.D
Acq On : 23 May 2022 10:44
Operator : SY/VA
Sample : N2925-05
Misc : 4.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY07

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/24/2022
Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 24 01:28:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

