




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023246.D
Acq On : 23 May 2022 13:33
Operator : SY/VA
Sample : N2926-11
Misc : 4.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY20

Manual IntegrationsAPPROVED

Quant Time: May 24 01:29:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/24/2022
Supervised By :Mahesh Dadoda 05/25/2022

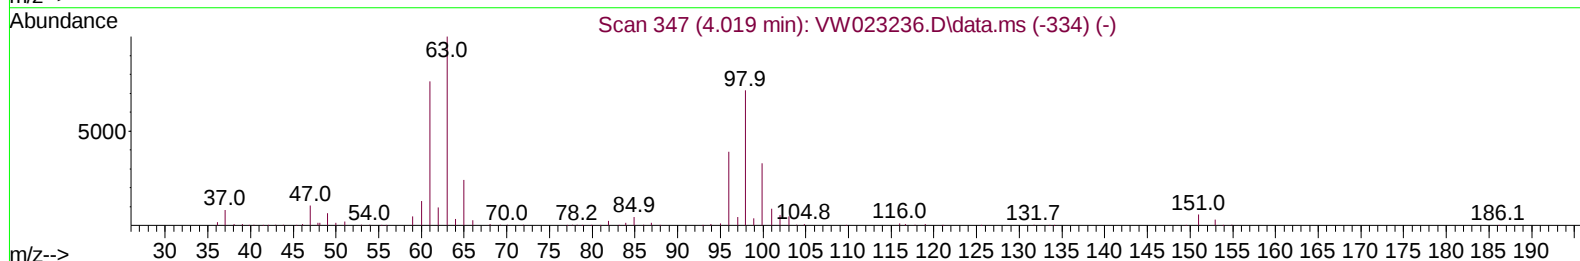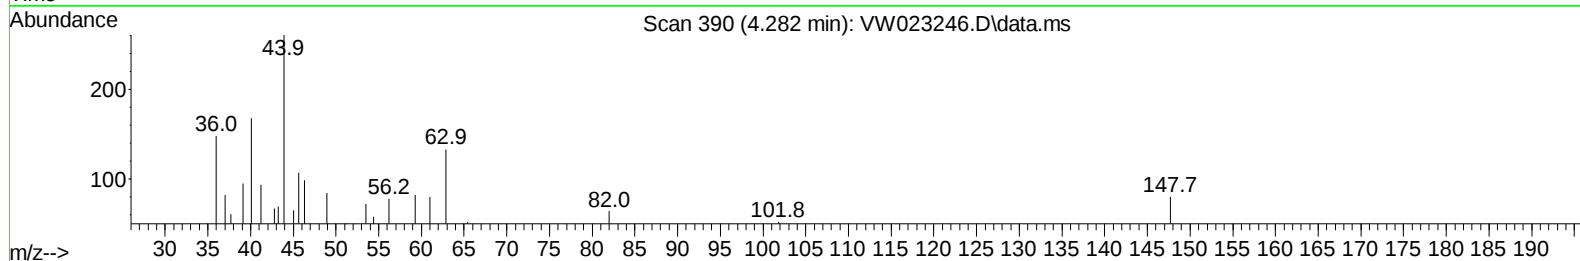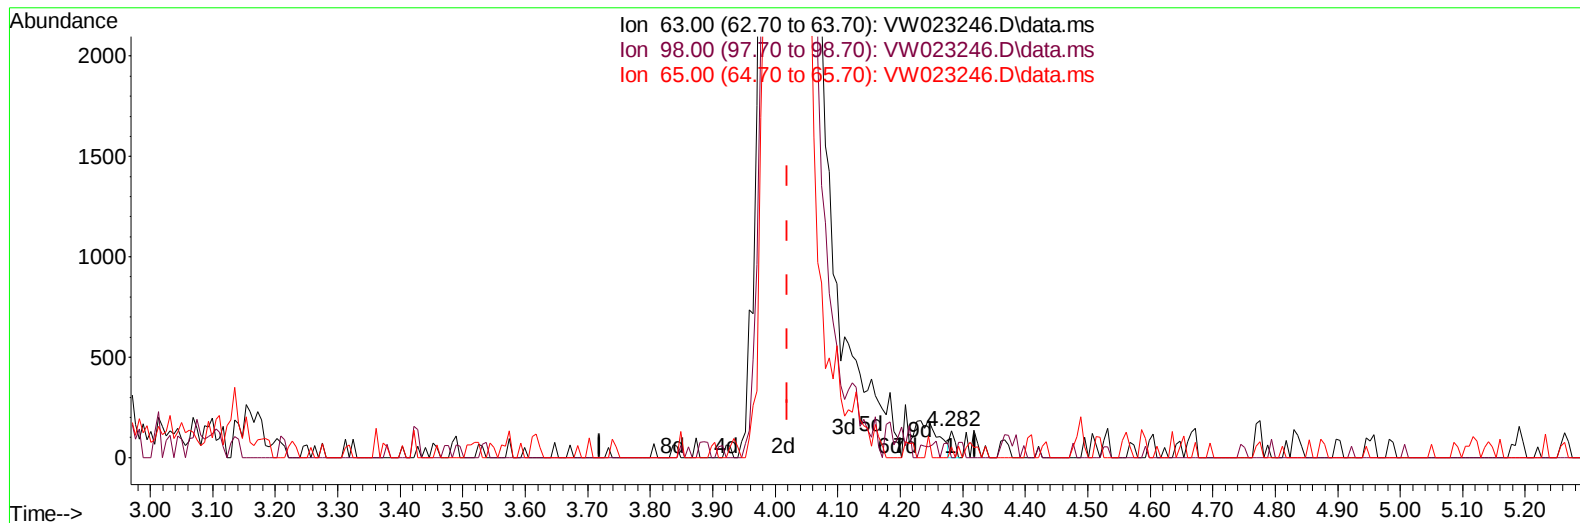

TIC: VW023246.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.282min (+ 0.262) 0.01 ug/L

response 77

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	66.23
65.00	23.30	24.68
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023246.D
 Acq On : 23 May 2022 13:33
 Operator : SY/VA
 Sample : N2926-11
 Misc : 4.34g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY20

Manual IntegrationsAPPROVED

Quant Time: May 24 01:29:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/24/2022
 Supervised By :Mahesh Dadoda 05/25/2022

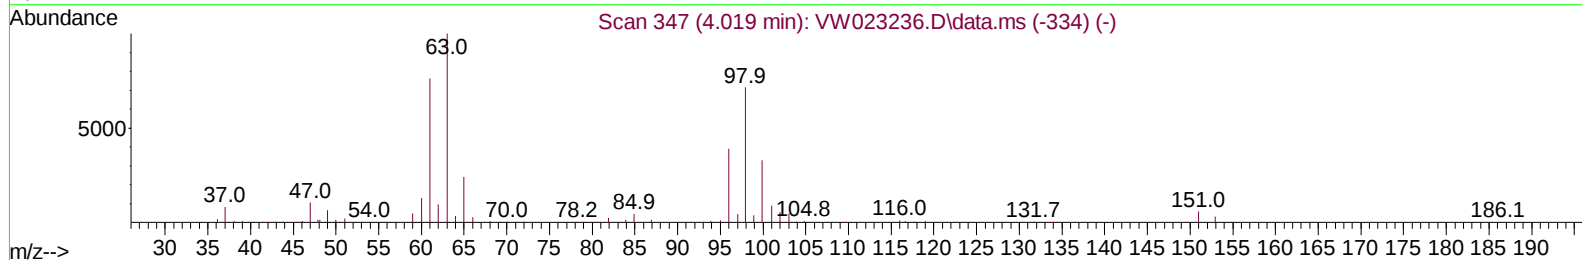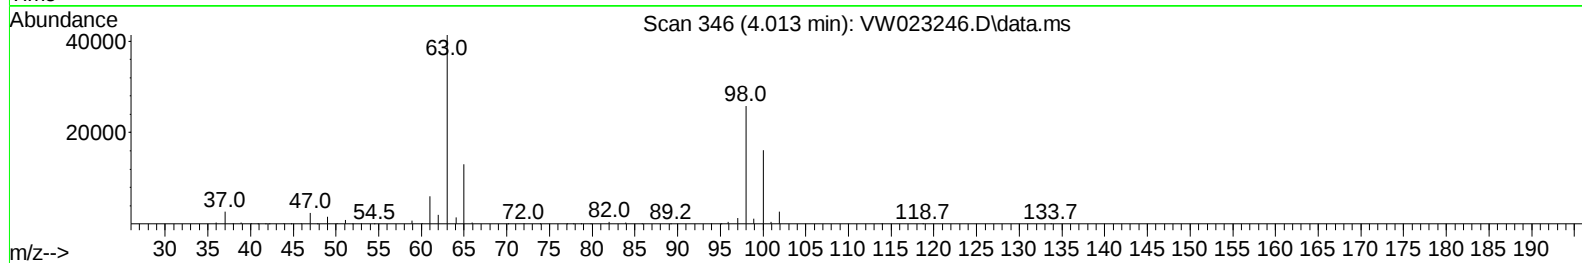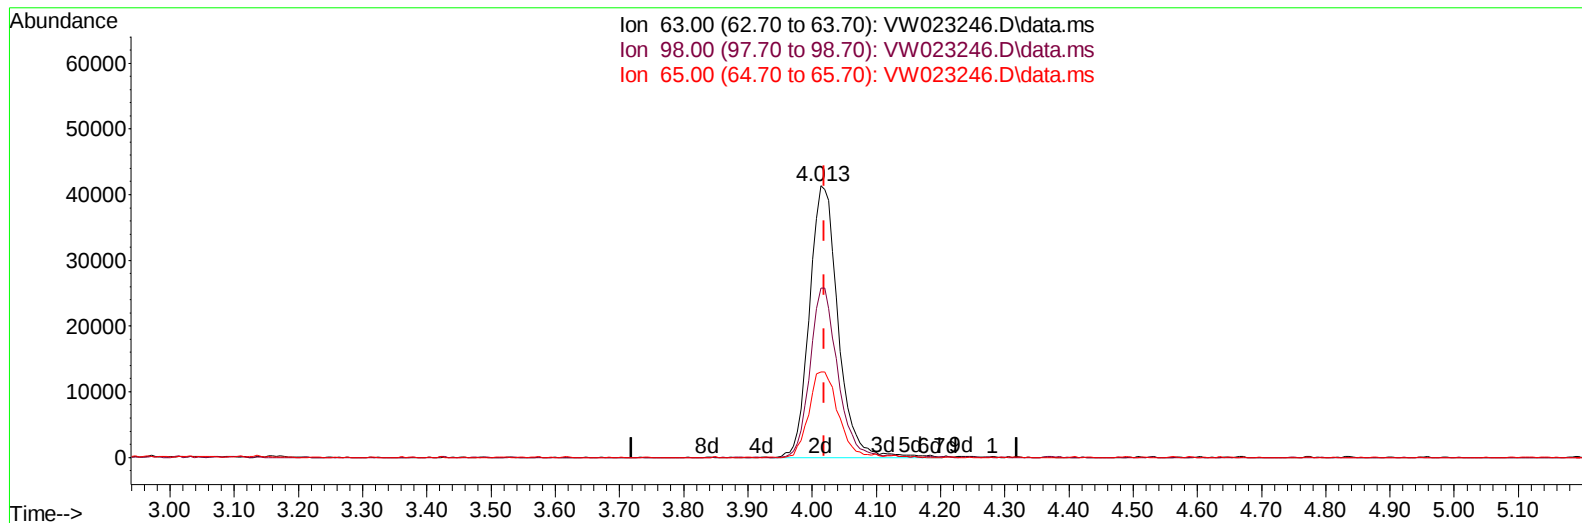

TIC: VW023246.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 14.52 ug/L m

response 127915

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.04#
65.00	23.30	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
 Data File : VW023246.D
 Acq On : 23 May 2022 13:33
 Operator : SY/VA
 Sample : N2926-11
 Misc : 4.34g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY20

Manual IntegrationsAPPROVED

Quant Time: May 24 01:29:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 24 01:27:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/24/2022
 Supervised By :Mahesh Dadoda 05/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	332370	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	304470	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	116031	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	132109	19.373	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.480%	
7) Chloroethane-d5	2.885	69	92919	20.945	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.760%	
11) 1,1-Dichloroethene-d2	4.013	63	127915m	14.518	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	58.080%	
21) 2-Butanone-d5	7.074	46	60698	46.816	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	93.640%	
24) Chloroform-d	7.653	84	238083	24.450	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	8.305	65	145095	27.168	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	108.680%	
32) Benzene-d6	8.275	84	439849	25.063	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	100.240%	
36) 1,2-Dichloropropane-d6	9.275	67	139197	28.236	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	112.960%	
41) Toluene-d8	10.323	98	399001	23.536	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	94.160%	
43) trans-1,3-Dichloroprop...	10.579	79	50858	22.406	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.640%	
47) 2-Hexanone-d5	10.921	63	44582	47.374	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	94.740%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	125372	27.286	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	109.160%	
66) 1,2-Dichlorobenzene-d4	13.853	152	104652	25.801	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	103.200%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052322\
Data File : VW023246.D
Acq On : 23 May 2022 13:33
Operator : SY/VA
Sample : N2926-11
Misc : 4.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY20

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/24/2022
Supervised By :Mahesh Dadoda 05/25/2022

Quant Time: May 24 01:29:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 24 01:27:20 2022
Response via : Initial Calibration

