




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052324\
 Data File : VW028705.D
 Acq On : 23 May 2024 14:18
 Operator : SY/MD
 Sample : P2549-06
 Misc : 3.63g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH623

Manual IntegrationsAPPROVED

Quant Time: May 31 06:50:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 29 23:53:47 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/24/2024
 Supervised By :Mahesh Dadoda 05/24/2024

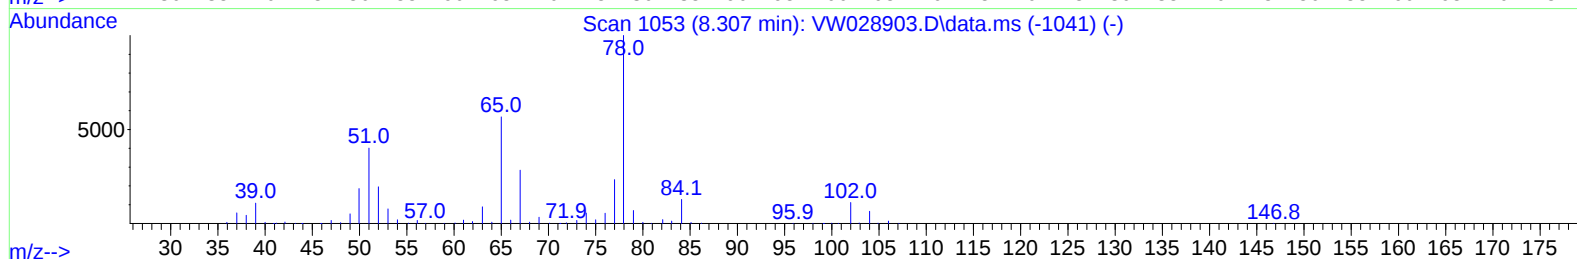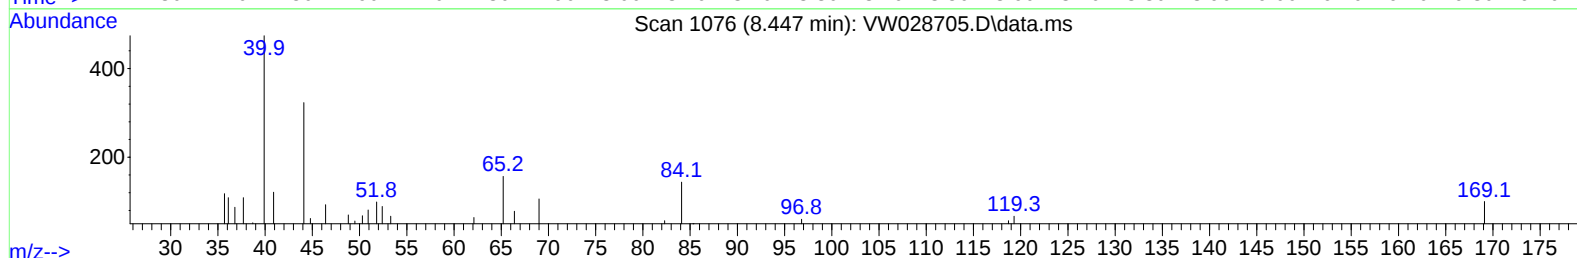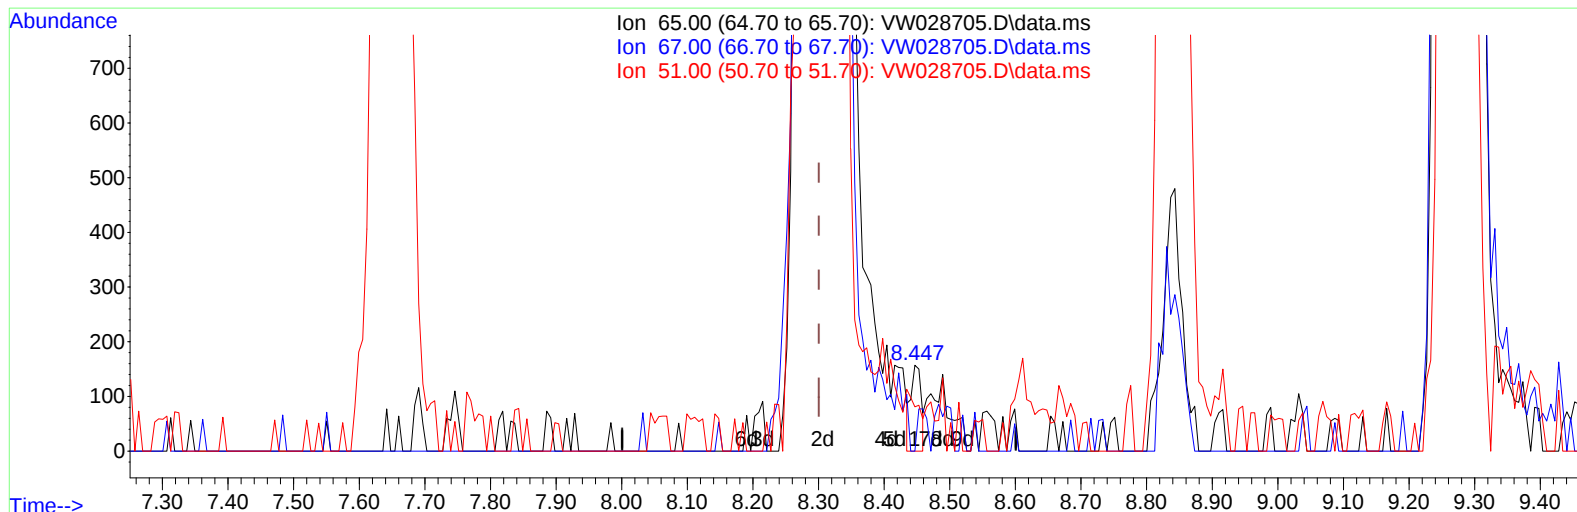

TIC: VW028705.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.447min (+ 0.146) 0.02 ug/L

response 172

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.60	45.35
51.00	101.70	92.44
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052324\
 Data File : VW028705.D
 Acq On : 23 May 2024 14:18
 Operator : SY/MD
 Sample : P2549-06
 Misc : 3.63g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH623

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/24/2024
 Supervised By :Mahesh Dadoda 05/24/2024

Quant Time: May 24 00:18:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 24 00:17:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	546823	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	374066	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	92809	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	168157	16.194	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	64.760%	
7) Chloroethane-d5	2.899	69	142865	17.969	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.880%	
11) 1,1-Dichloroethene-d2	4.021	65	77116	17.775	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	71.120%	
21) 2-Butanone-d5	7.081	46	55686	20.555	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	41.120%	
24) Chloroform-d	7.648	84	347632	20.345	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	81.400%	
26) 1,2-Dichloroethane-d4	8.306	65	184226m	18.833	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	75.320%	
32) Benzene-d6	8.270	84	664209	26.614	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	106.440%	
36) 1,2-Dichloropropane-d6	9.270	67	209955	27.957	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	111.840%	
41) Toluene-d8	10.324	98	526216	23.809	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	95.240%	
43) trans-1,3-Dichloroprop...	10.574	79	54072	17.898	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.600%	
47) 2-Hexanone-d5	10.922	63	34938	26.974	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	53.940%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	106454	16.905	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	67.600%	
66) 1,2-Dichlorobenzene-d4	13.854	152	71097	20.099	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	80.400%	
Target Compounds						
16) Methylene chloride	4.917	84	31001	3.666	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052324\
Data File : VW028705.D
Acq On : 23 May 2024 14:18
Operator : SY/MD
Sample : P2549-06
Misc : 3.63g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH623

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/24/2024
Supervised By :Mahesh Dadoda 05/24/2024

Quant Time: May 24 00:18:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 00:17:02 2024
Response via : Initial Calibration

