

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023280.D
 Acq On : 24 May 2022 18:24
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK480

Quant Time: May 25 00:56:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 00:48:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	297305	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	309597	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	149908	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	101461	16.634	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.520%
7) Chloroethane-d5	2.879	69	72468	18.262	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.040%
11) 1,1-Dichloroethene-d2	4.013	63	98331	12.476	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.920%
21) 2-Butanone-d5	7.080	46	55877	48.181	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.360%
24) Chloroform-d	7.647	84	187259	21.498	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	8.305	65	109644	22.951	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.800%
32) Benzene-d6	8.275	84	361581	20.262	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.040%
36) 1,2-Dichloropropane-d6	9.275	67	106545	21.255	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.040%
41) Toluene-d8	10.323	98	341061	19.785	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.160%
43) trans-1,3-Dichloroprop...	10.579	79	45446	19.690	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.760%
47) 2-Hexanone-d5	10.927	63	43203	45.148	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.300%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	103294	22.108	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	117090	22.344	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.360%
Target Compounds					Qvalue	
13) Acetone	4.129	43	3100	3.570	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023280.D
Acq On : 24 May 2022 18:24
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK480

Quant Time: May 25 00:56:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 00:48:22 2022
Response via : Initial Calibration

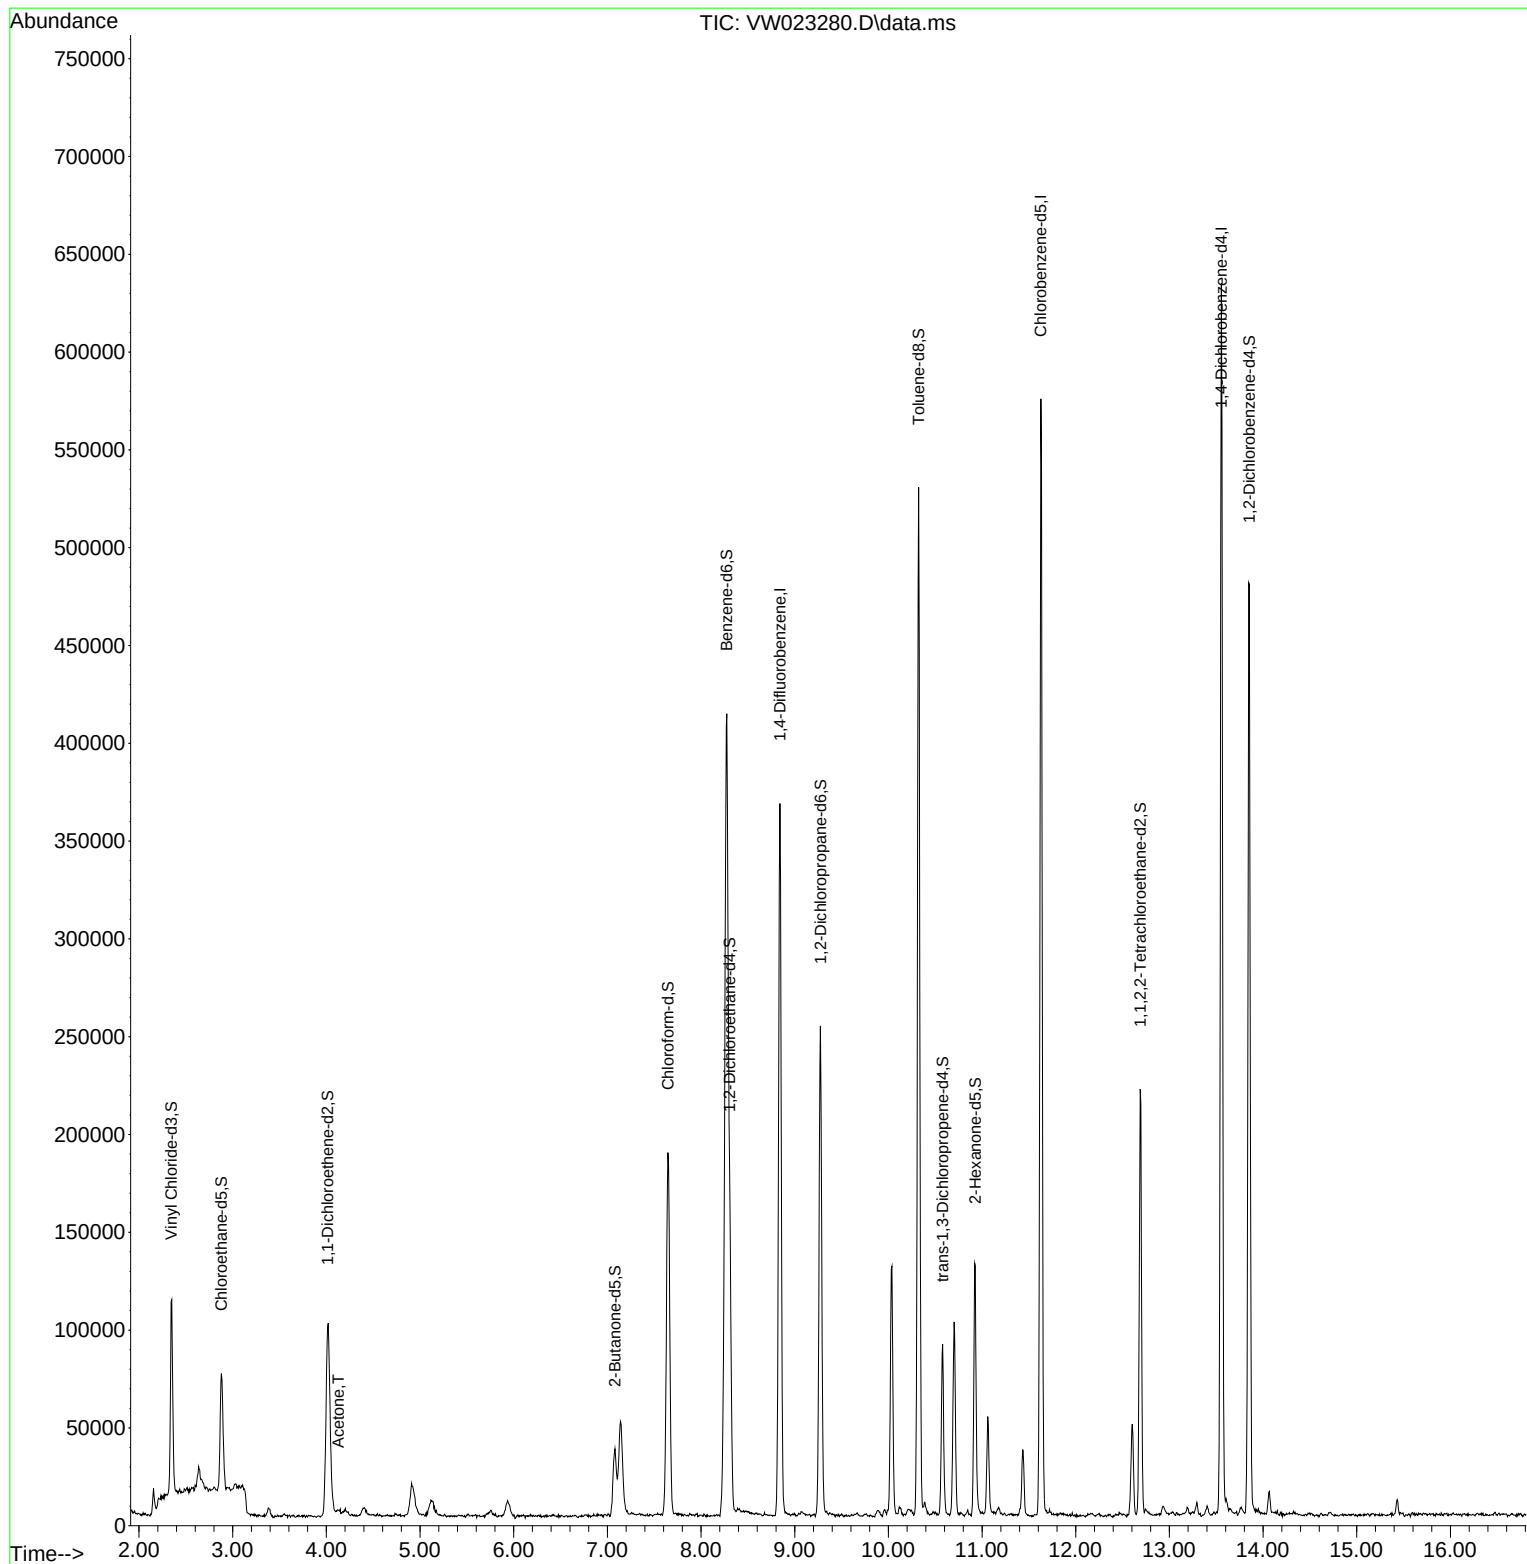

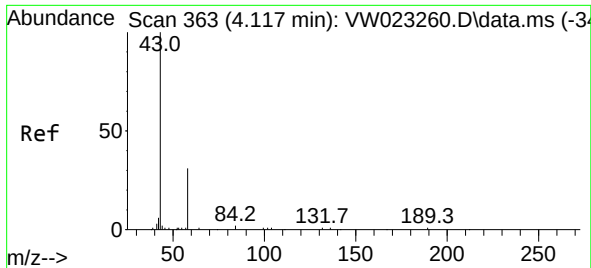

#13

Acetone

Concen: 3.570 ug/L

RT: 4.129 min Scan# 30

Delta R.T. 0.012 min

Lab File: VW023280.D

Acq: 24 May 2022 18:24

Instrument :

MSVOA_W

ClientSampleId :

VIBLK480

Tgt Ion: 43 Resp: 3100

Ion Ratio Lower Upper

43 100

58 27.9 0.0 64.0

