

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023298.D
 Acq On : 25 May 2022 02:50
 Operator : SY/VA
 Sample : N2995-11
 Misc : 3.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 25 06:00:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	333922	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	294121	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	115424	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	139747	20.398	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	81.600%	
7) Chloroethane-d5	2.879	69	106920	23.989	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	95.960%	
11) 1,1-Dichloroethene-d2	4.013	63	131139	14.814	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	59.240%	
21) 2-Butanone-d5	7.074	46	105006	80.614	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	161.220%#	
24) Chloroform-d	7.647	84	286753	29.311	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	117.240%	
26) 1,2-Dichloroethane-d4	8.299	65	178995	33.359	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	133.440%#	
32) Benzene-d6	8.275	84	483768	28.536	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	114.160%	
36) 1,2-Dichloropropane-d6	9.275	67	163566	34.347	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	137.400%#	
41) Toluene-d8	10.323	98	362333	22.125	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	88.520%	
43) trans-1,3-Dichloroprop...	10.573	79	59378	27.080	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	108.320%	
47) 2-Hexanone-d5	10.921	63	78692	86.562	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	173.120%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	180364	40.635	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	162.560%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	122050	30.249	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	121.000%#	
Target Compounds					Qvalue	
13) Acetone	4.123	43	26128	26.792	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023298.D
Acq On : 25 May 2022 02:50
Operator : SY/VA
Sample : N2995-11
Misc : 3.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 25 06:00:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

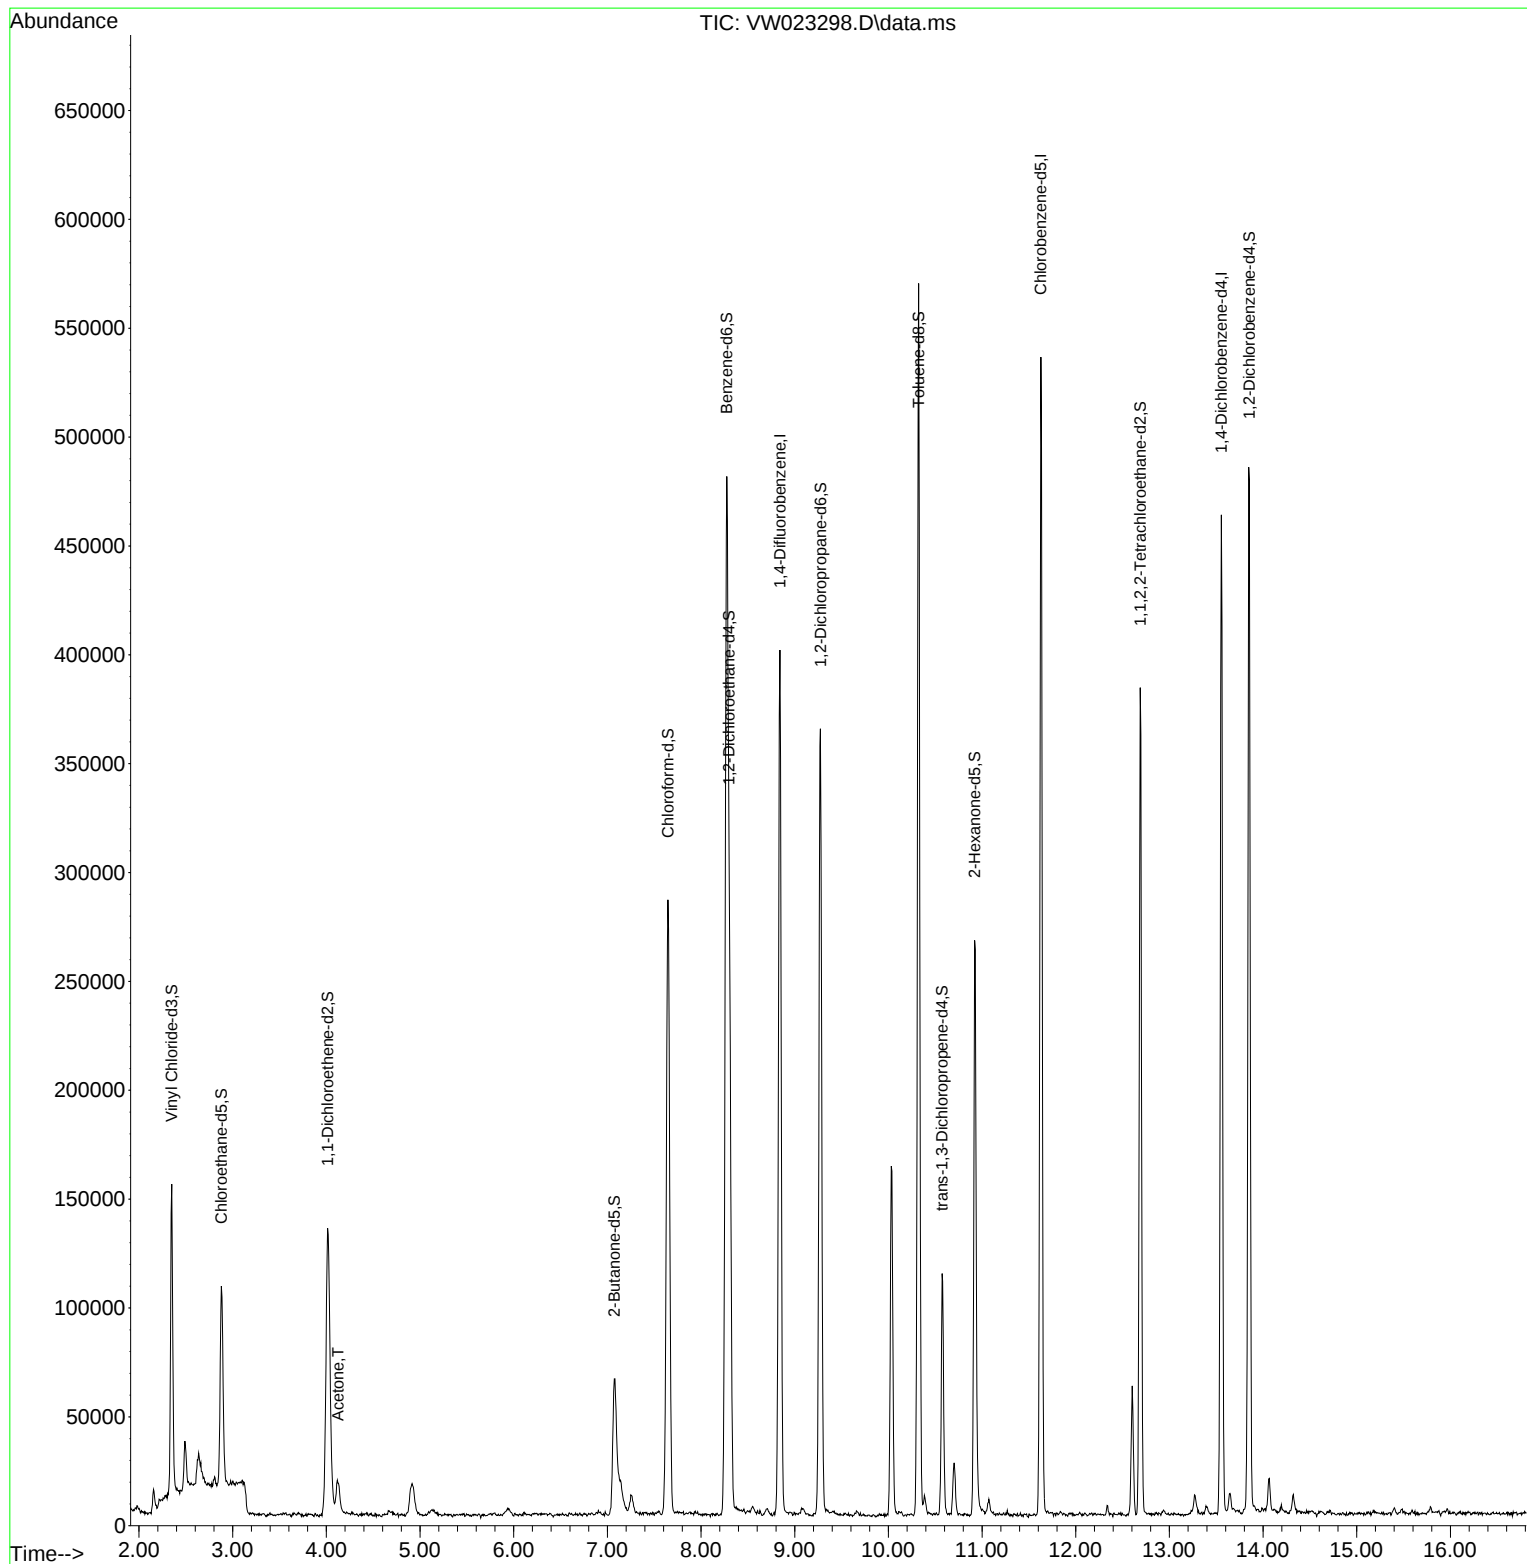

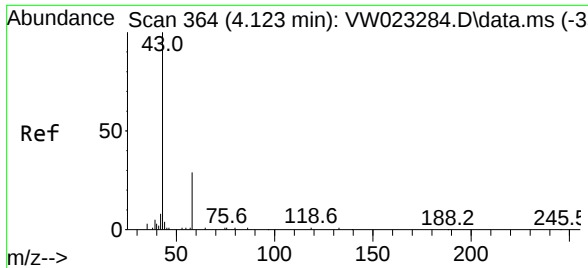

#13
 Acetone
 Concen: 26.792 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW023298.D
 Acq: 25 May 2022 02:50

Instrument :
 MSVOA_W
 ClientSampleId :

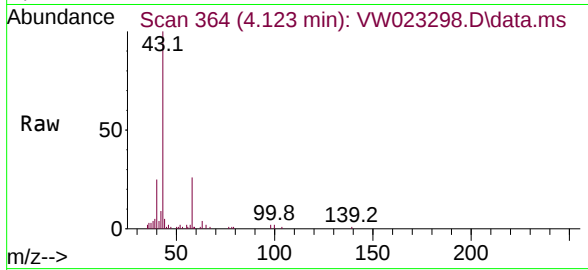

Tgt Ion:	43	Resp:	26128
Ion	Ratio	Lower	Upper
43	100		
58	29.0	0.0	64.0

