




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023281.D
 Acq On : 24 May 2022 18:48
 Operator : SY/VA
 Sample : N2976-01
 Misc : 4.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY22

Manual IntegrationsAPPROVED

Quant Time: May 25 00:56:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 00:48:22 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

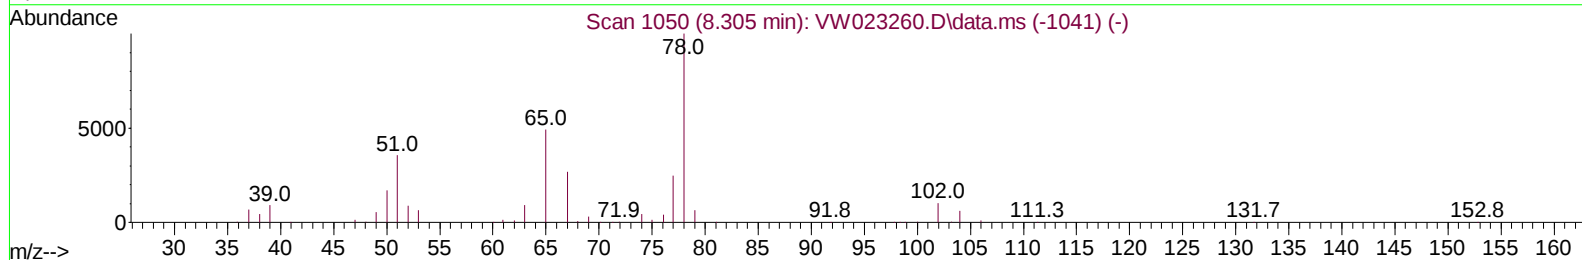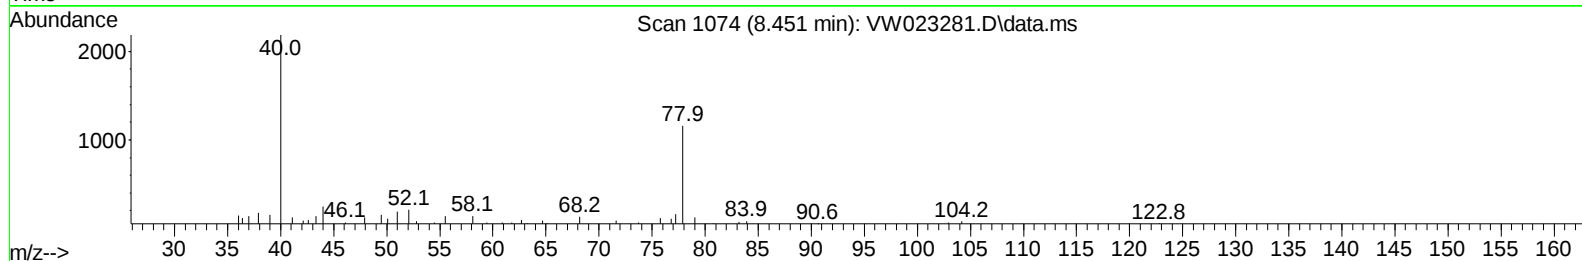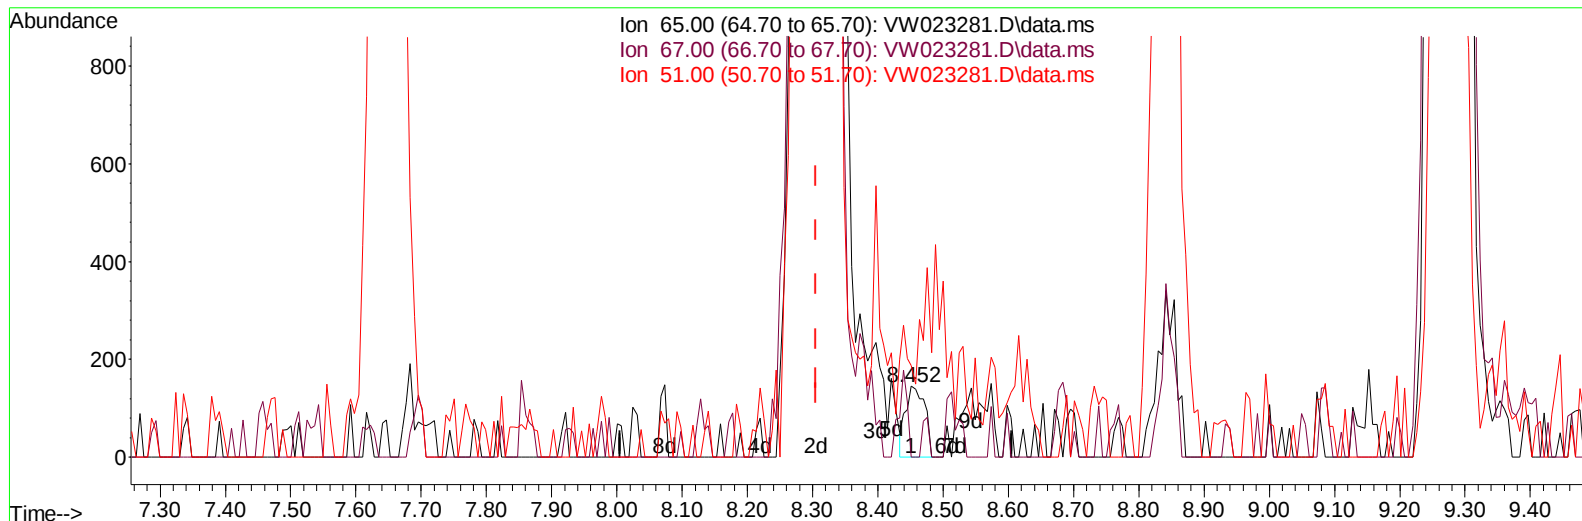

TIC: VW023281.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.451min (+ 0.146) 0.05 ug/L

response 294

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	55.78
51.00	92.30	71.09
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023281.D
 Acq On : 24 May 2022 18:48
 Operator : SY/VA
 Sample : N2976-01
 Misc : 4.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY22

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 00:56:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 00:48:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	358282	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	344722	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	148602	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	123548	16.808	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.240%	
7) Chloroethane-d5	2.885	69	112677	23.562	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	94.240%	
11) 1,1-Dichloroethene-d2	4.019	63	128230	13.501	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	54.000%	
21) 2-Butanone-d5	7.080	46	37445	26.792	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	53.580%	
24) Chloroform-d	7.647	84	260720	24.838	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	99.360%	
26) 1,2-Dichloroethane-d4	8.305	65	152458m	26.482	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	105.920%	
32) Benzene-d6	8.275	84	462956	23.300	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	93.200%	
36) 1,2-Dichloropropane-d6	9.275	67	150492	26.963	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	107.840%	
41) Toluene-d8	10.323	98	410164	21.369	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	85.480%	
43) trans-1,3-Dichloroprop...	10.573	79	53879	20.965	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	83.880%	
47) 2-Hexanone-d5	10.921	63	25801	24.215	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	48.440%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	136916	26.319	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	105.280%	
66) 1,2-Dichlorobenzene-d4	13.853	152	132263	25.462	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	101.840%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023281.D
Acq On : 24 May 2022 18:48
Operator : SY/VA
Sample : N2976-01
Misc : 4.95g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY22

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 00:56:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 00:48:22 2022
Response via : Initial Calibration

