




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023287.D
Acq On : 24 May 2022 22:25
Operator : SY/VA
Sample : N2926-13RE
Misc : 2.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY23RE

Manual IntegrationsAPPROVED

Quant Time: May 25 04:09:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

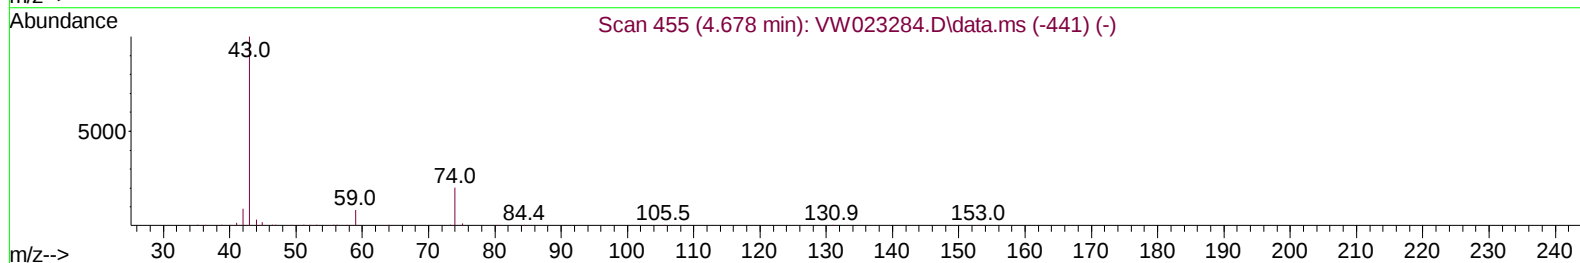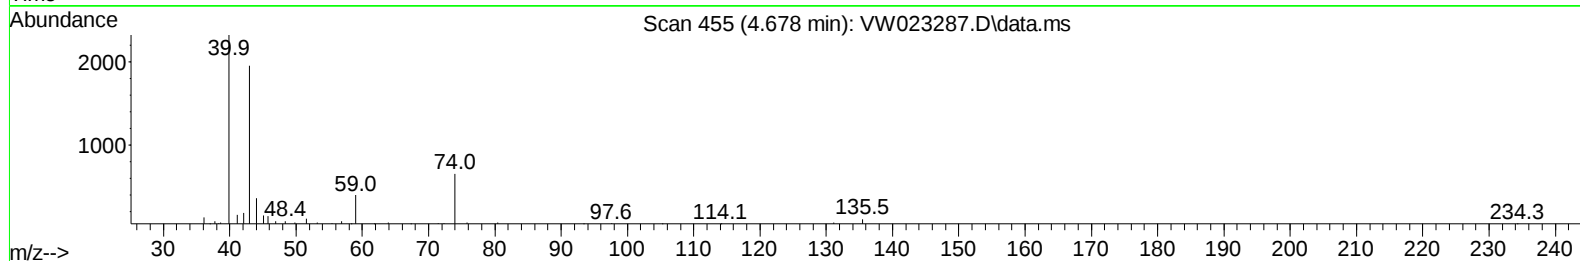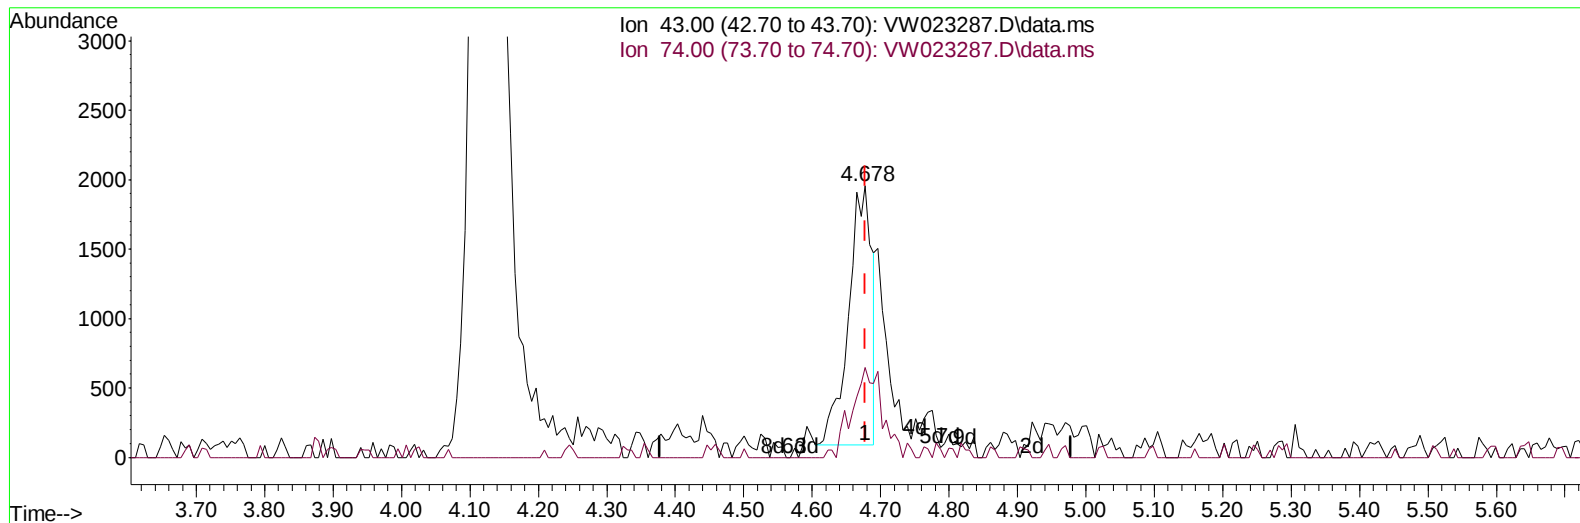

TIC: VW023287.D\data.ms

(15) Methyl Acetate (T)

4.678min (+ 0.000) 2.71 ug/L

response 4435

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.40	24.98
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023287.D
 Acq On : 24 May 2022 22:25
 Operator : SY/VA
 Sample : N2926-13RE
 Misc : 2.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY23RE

Manual IntegrationsAPPROVED

Quant Time: May 25 04:09:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

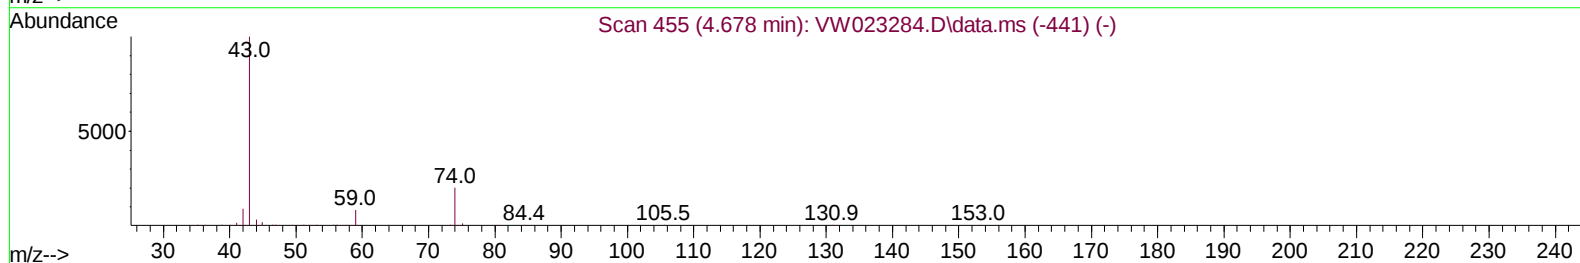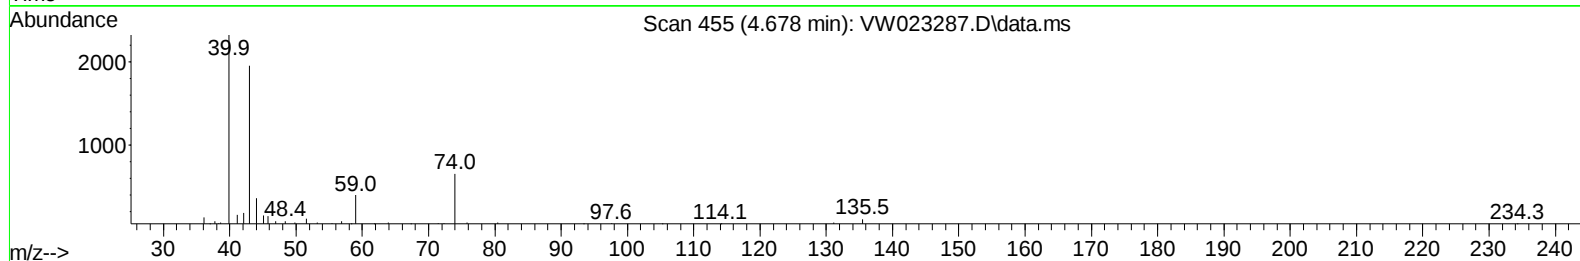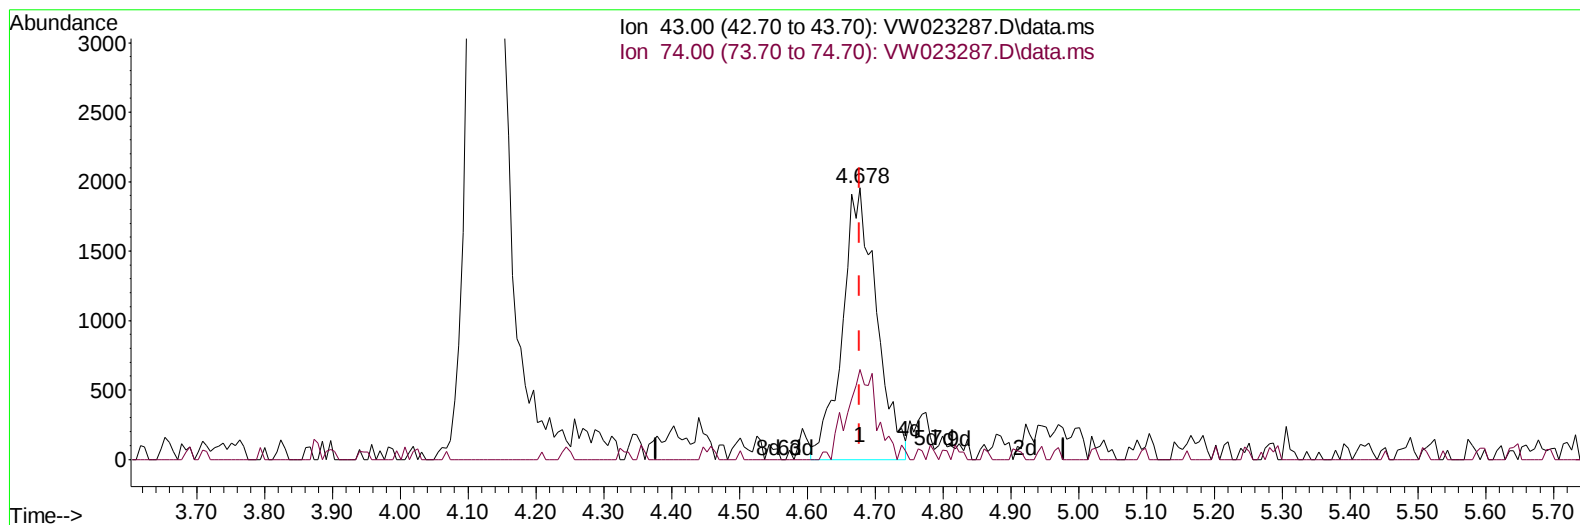

TIC: VW023287.D\data.ms

(15) Methyl Acetate (T)

4.678min (+ 0.000) 4.16 ug/L m

response 6817

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	27.40	16.25#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023287.D
 Acq On : 24 May 2022 22:25
 Operator : SY/VA
 Sample : N2926-13RE
 Misc : 2.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY23RE

Manual IntegrationsAPPROVED

Quant Time: May 25 04:09:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

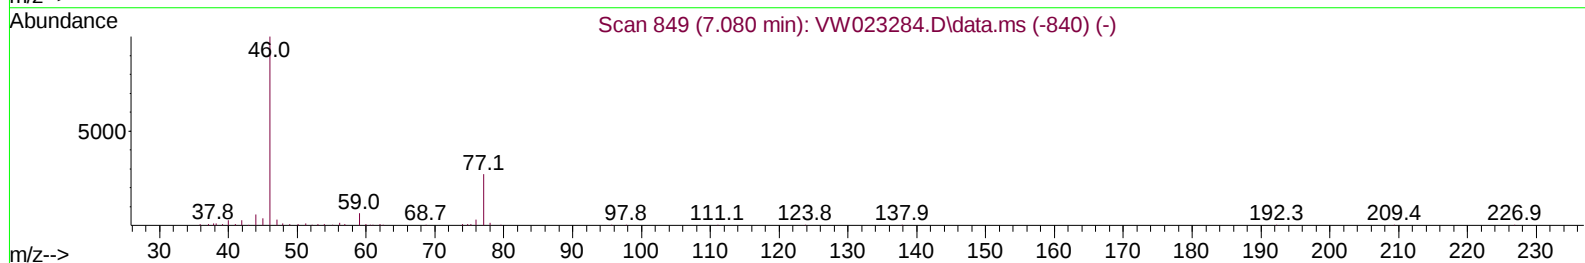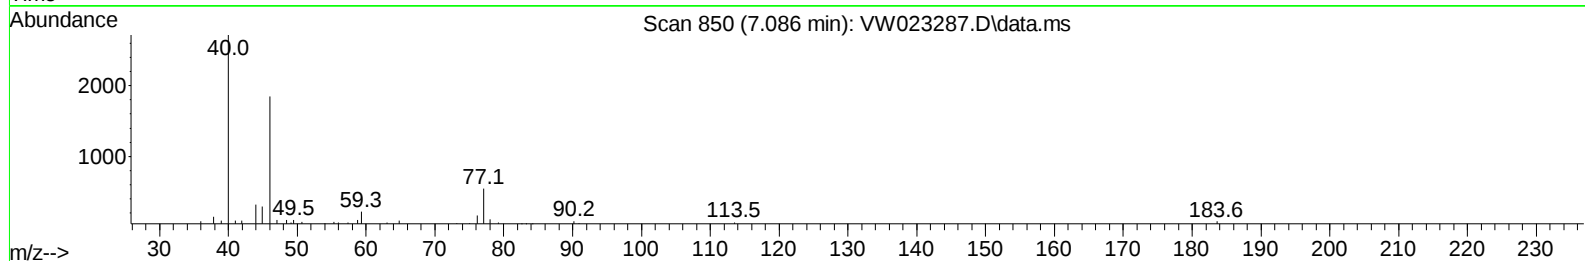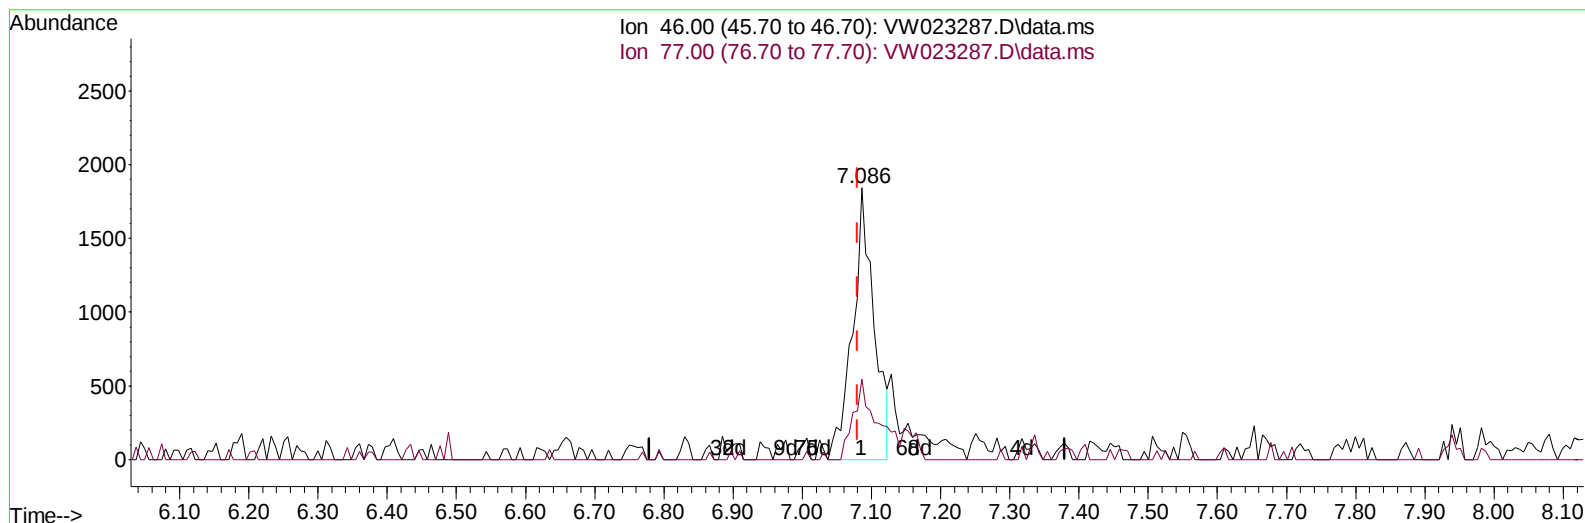

TIC: VW023287.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 3.64 ug/L

response 3966

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	33.31
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023287.D
 Acq On : 24 May 2022 22:25
 Operator : SY/VA
 Sample : N2926-13RE
 Misc : 2.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY23RE

Manual IntegrationsAPPROVED

Quant Time: May 25 04:09:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

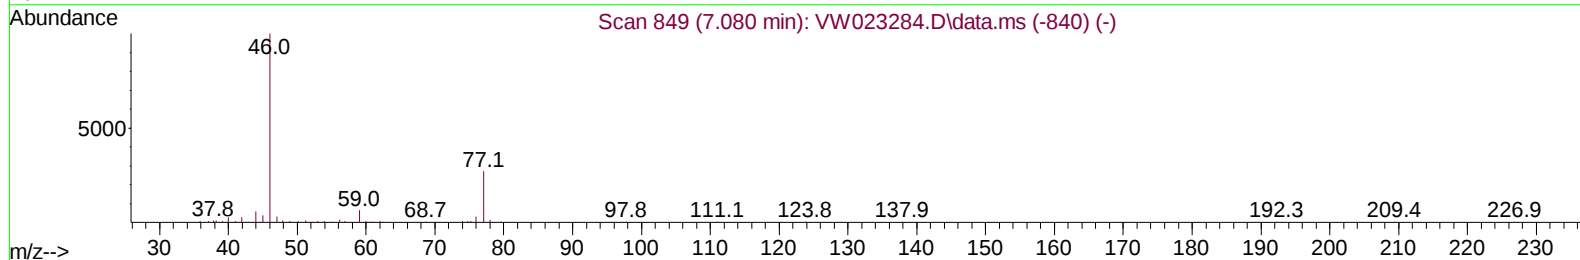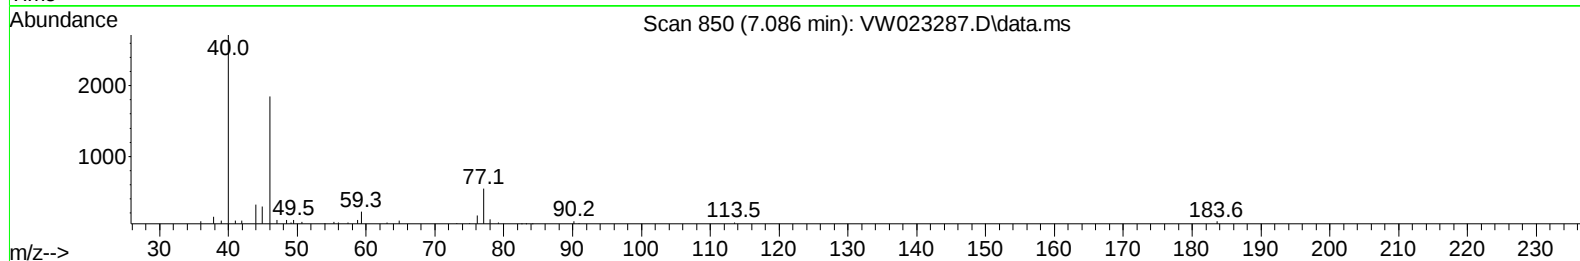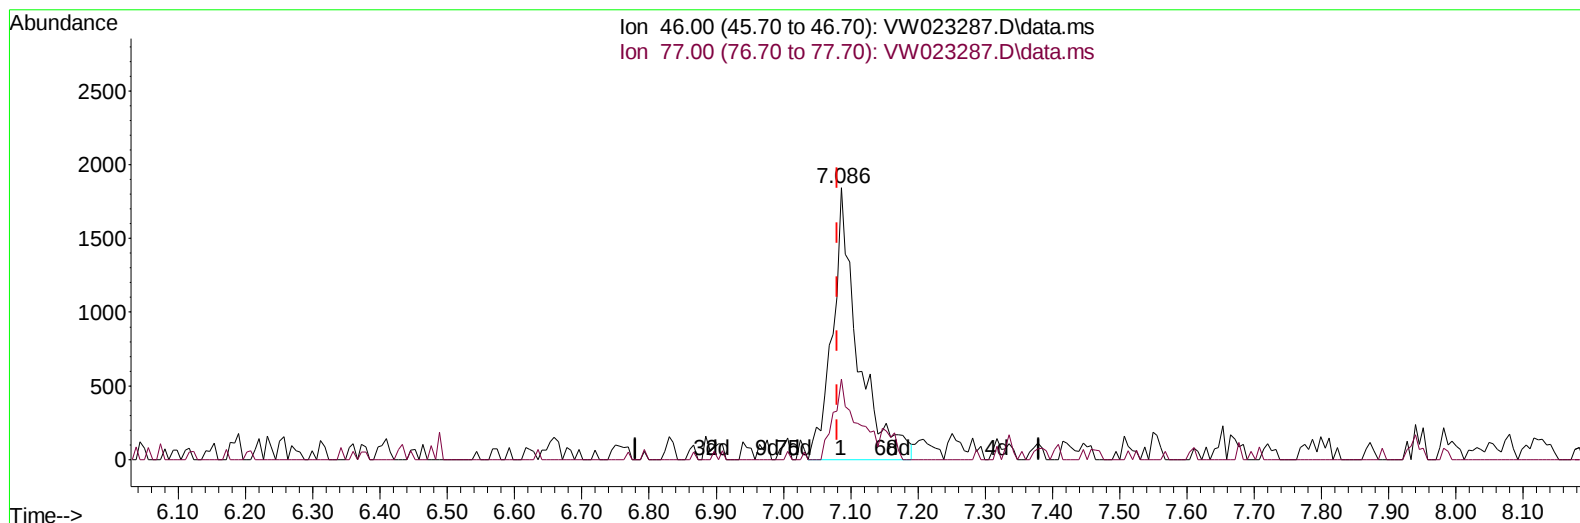

TIC: VW023287.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 4.45 ug/L m

response 4850

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	27.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023287.D
Acq On : 24 May 2022 22:25
Operator : SY/VA
Sample : N2926-13RE
Misc : 2.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY23RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 04:09:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

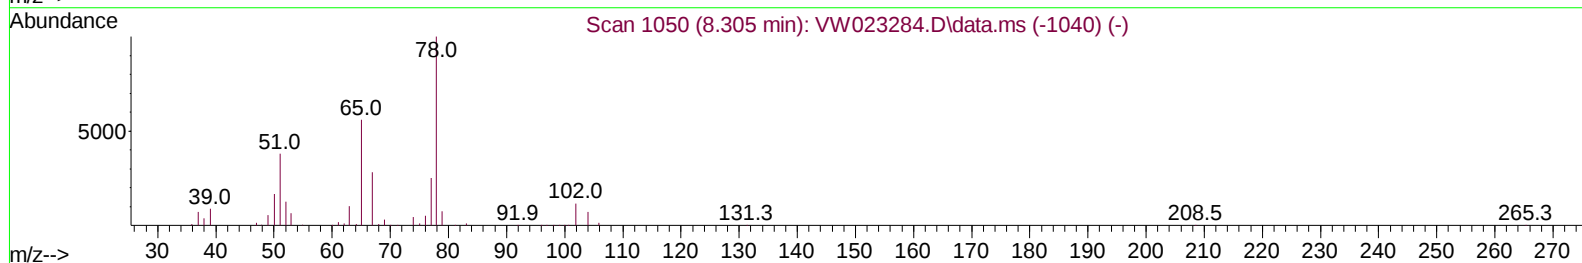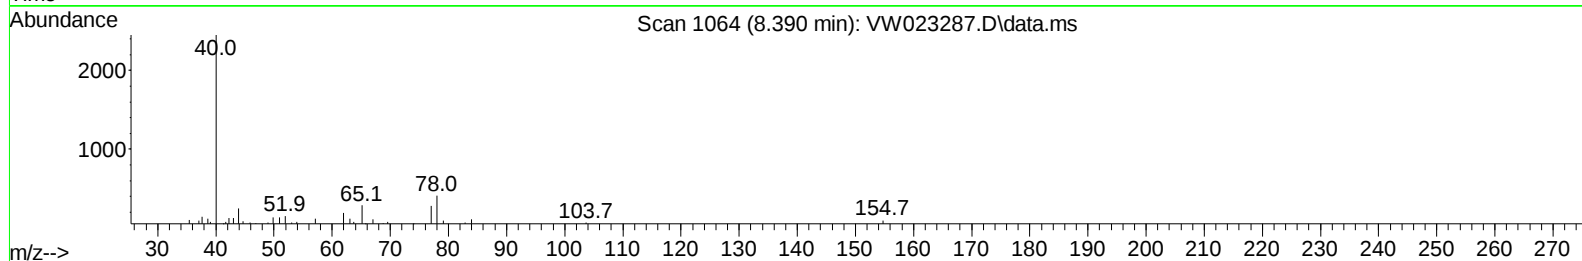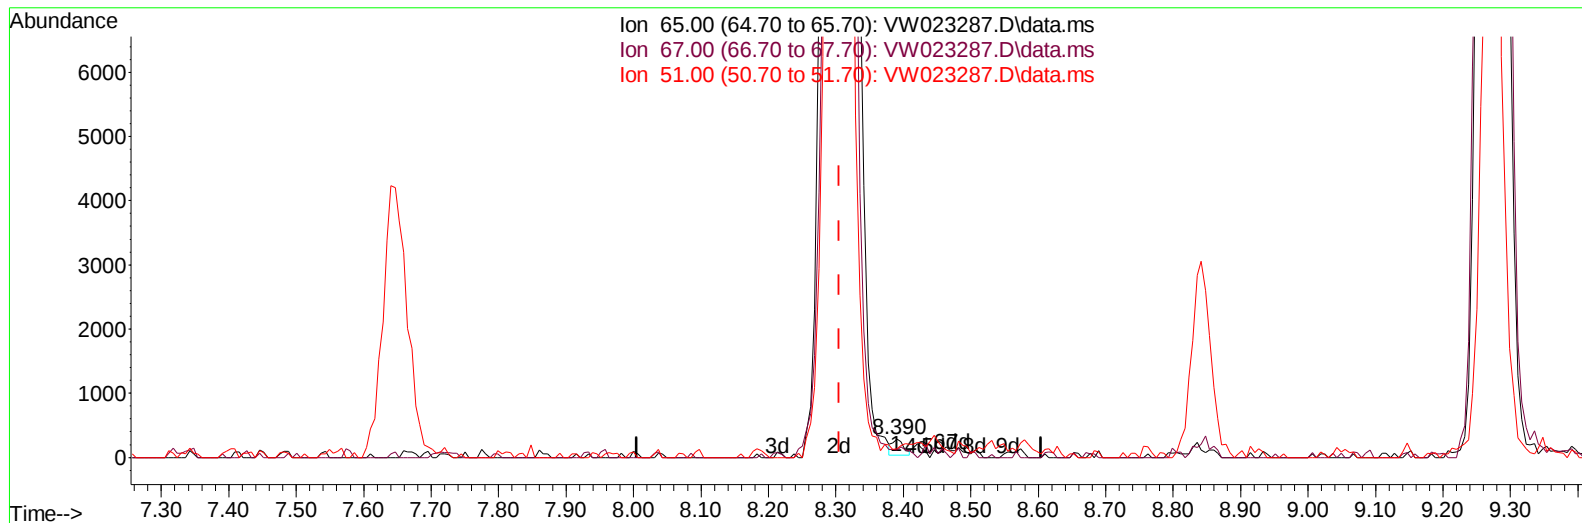

TIC: VW023287.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.390min (+ 0.085) 0.07 ug/L

response 292

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	55.48
51.00	92.30	88.36
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023287.D
 Acq On : 24 May 2022 22:25
 Operator : SY/VA
 Sample : N2926-13RE
 Misc : 2.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY23RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 04:09:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

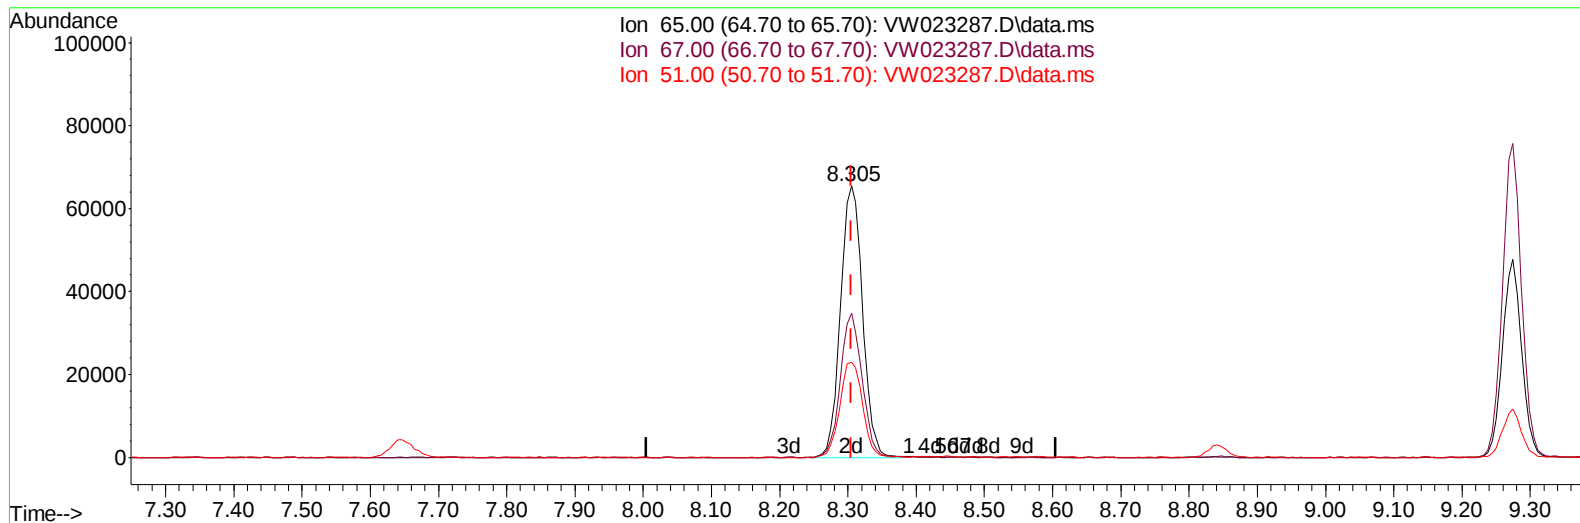

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023287.D
 Acq On : 24 May 2022 22:25
 Operator : SY/VA
 Sample : N2926-13RE
 Misc : 2.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXY23RE

Manual IntegrationsAPPROVED

Quant Time: May 25 04:09:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		279133	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		204336	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		53978	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		132079	23.063	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	92.240%	
7) Chloroethane-d5	2.885	69		89514	24.026	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	96.120%	
11) 1,1-Dichloroethene-d2	4.013	63		117581	15.890	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	63.560%	
21) 2-Butanone-d5	7.086	46		4850m	4.454	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	8.900%#	
24) Chloroform-d	7.647	84		256086	31.314	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	125.240%	
26) 1,2-Dichloroethane-d4	8.305	65		146629m	32.691	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	130.760%#	
32) Benzene-d6	8.275	84		412880	35.056	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	140.240%#	
36) 1,2-Dichloropropane-d6	9.274	67		146846	44.386	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	177.560%#	
41) Toluene-d8	10.323	98		296609	26.070	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	104.280%	
43) trans-1,3-Dichloroprop...	10.579	79		16178	10.620	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	42.480%	
47) 2-Hexanone-d5	10.920	63		1526	2.416	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	4.840%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		112315	36.423	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	145.680%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		56408	29.895	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	119.560%	
Target Compounds							
						Qvalue	
13) Acetone	4.123	43		29824	36.584	ug/L	99
15) Methyl Acetate	4.678	43		6817m	4.162	ug/L	
46) Tetrachloroethene	10.860	164		2536	1.019	ug/L	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023287.D
Acq On : 24 May 2022 22:25
Operator : SY/VA
Sample : N2926-13RE
Misc : 2.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXY23RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 04:09:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

