


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023288.D
 Acq On : 24 May 2022 22:49
 Operator : SY/VA
 Sample : N2995-01
 Misc : 4.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 04:10:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

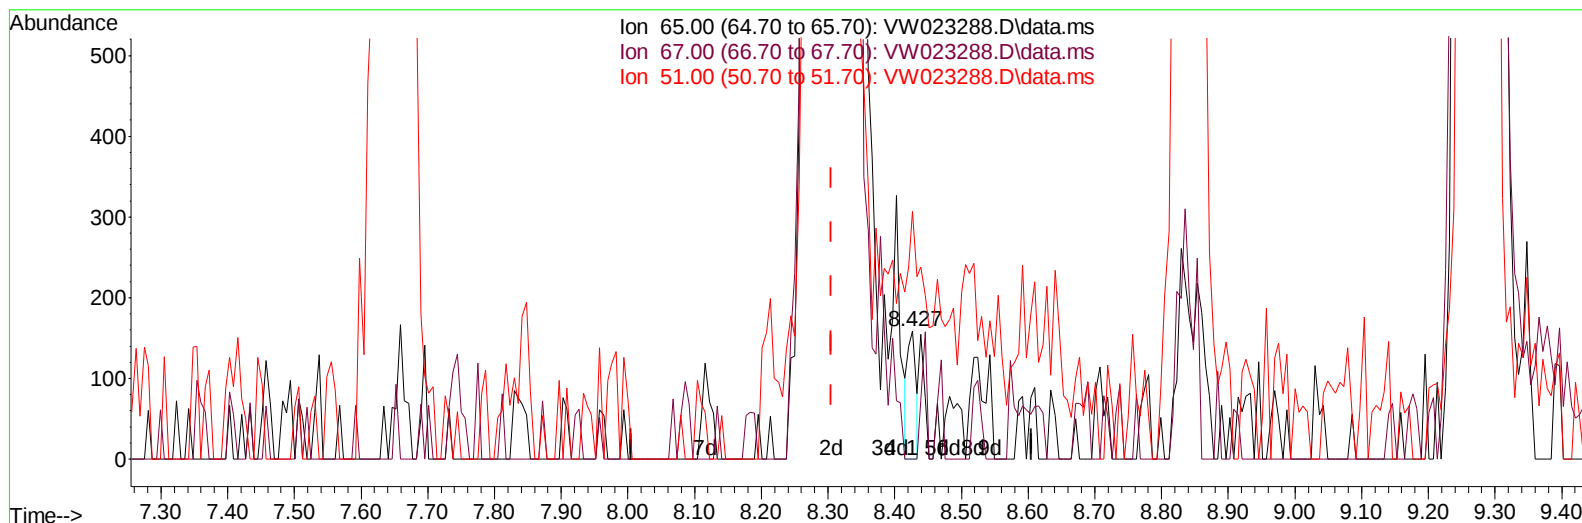




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023288.D
 Acq On : 24 May 2022 22:49
 Operator : SY/VA
 Sample : N2995-01
 Misc : 4.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 04:10:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

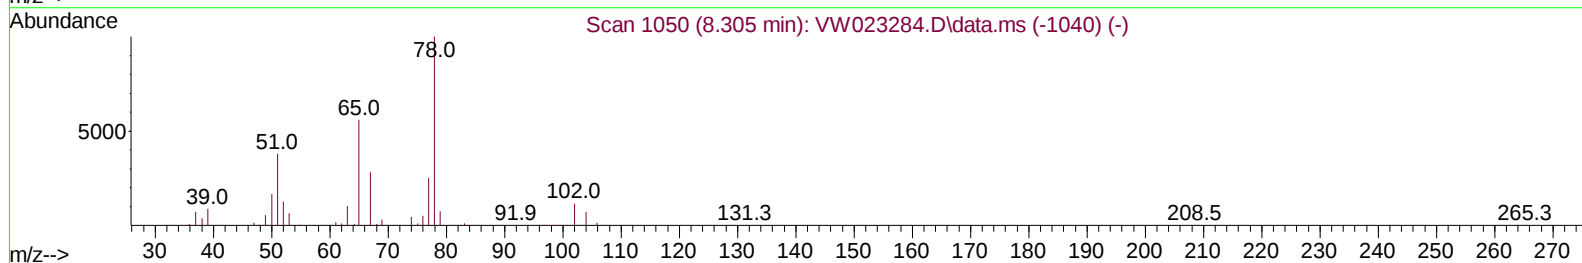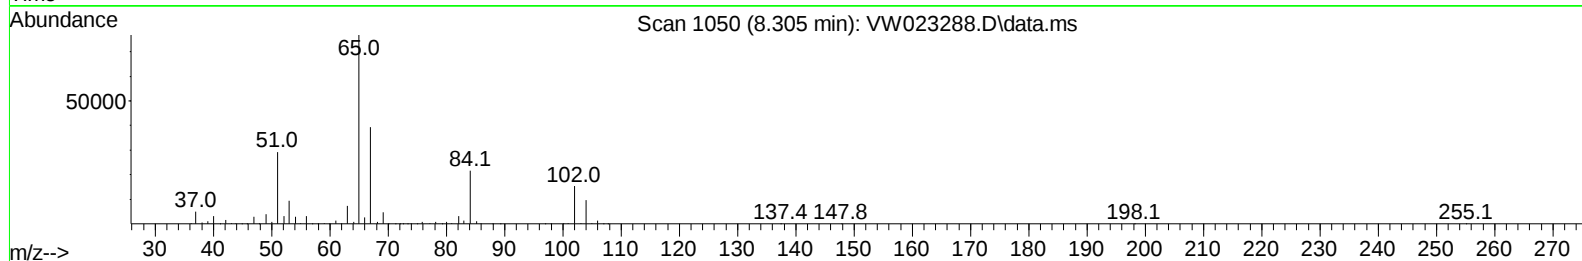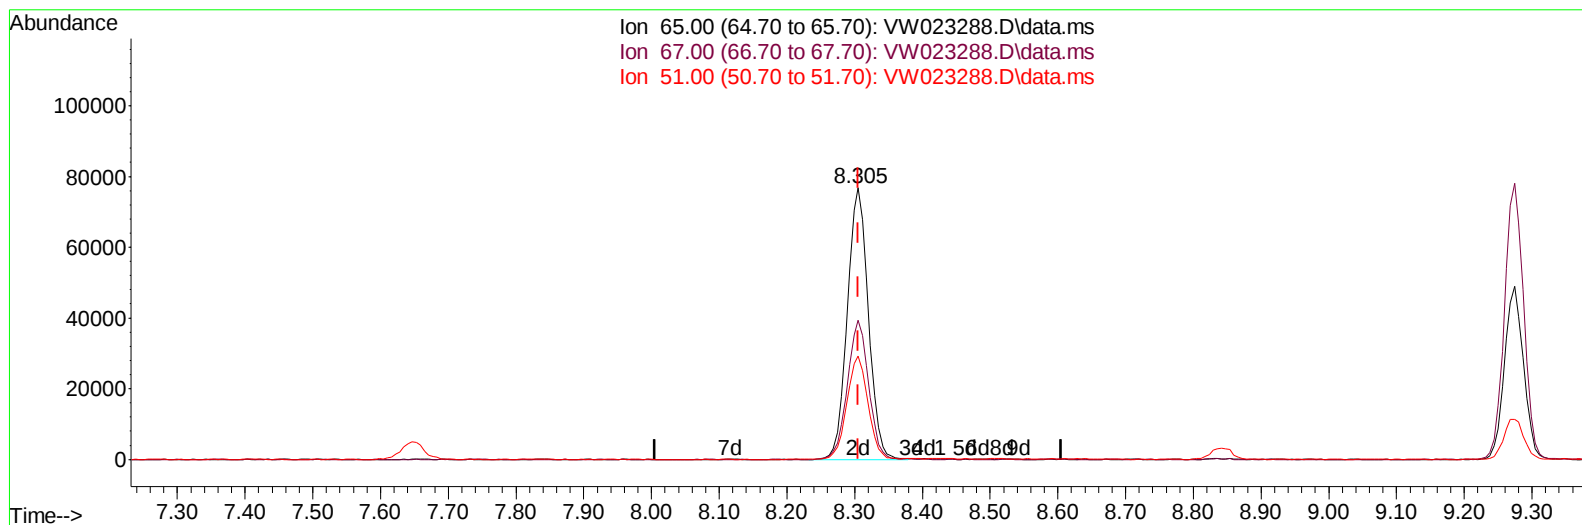

TIC: VW023288.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (0.000) 31.60 ug/L m

response 165469

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.05#
51.00	92.30	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023288.D
 Acq On : 24 May 2022 22:49
 Operator : SY/VA
 Sample : N2995-01
 Misc : 4.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 04:10:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		325861	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		280598	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		107980	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		131480	19.666	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	78.680%	
7) Chloroethane-d5	2.879	69		85591	19.679	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	78.720%	
11) 1,1-Dichloroethene-d2	4.013	63		125468	14.524	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	58.080%	
21) 2-Butanone-d5	7.074	46		105425	82.938	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	165.880%#	
24) Chloroform-d	7.647	84		266538	27.919	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	111.680%	
26) 1,2-Dichloroethane-d4	8.305	65		165469m	31.601	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	126.400%	
32) Benzene-d6	8.275	84		454306	28.090	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	112.360%	
36) 1,2-Dichloropropane-d6	9.274	67		154101	33.919	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	135.680%#	
41) Toluene-d8	10.323	98		370357	23.705	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	94.800%	
43) trans-1,3-Dichloroprop...	10.579	79		54501	26.054	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	104.200%	
47) 2-Hexanone-d5	10.920	63		77682	89.569	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	179.140%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		168433	39.776	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	159.120%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		108716	28.802	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	115.200%	
Target Compounds							
						Qvalue	
13) Acetone	4.123	43		19780	20.784	ug/L	99
42) Toluene	10.384	91		27846	1.503	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023288.D
Acq On : 24 May 2022 22:49
Operator : SY/VA
Sample : N2995-01
Misc : 4.60g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGQ4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 04:10:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

