




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023293.D
 Acq On : 25 May 2022 00:50
 Operator : SY/VA
 Sample : N2995-06
 Misc : 3.47g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ9

Manual IntegrationsAPPROVED

Quant Time: May 25 05:59:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

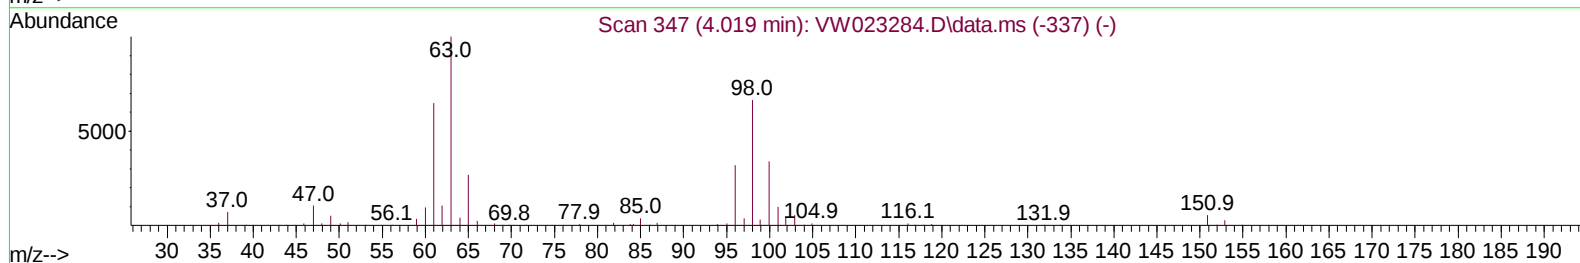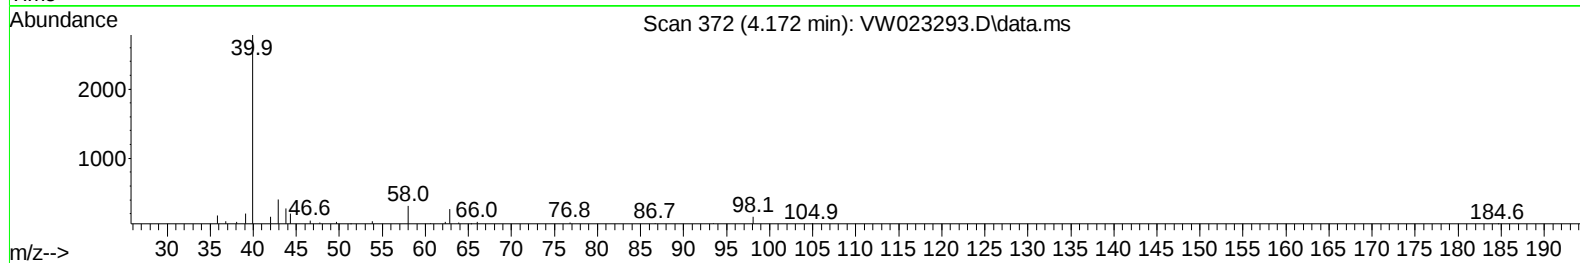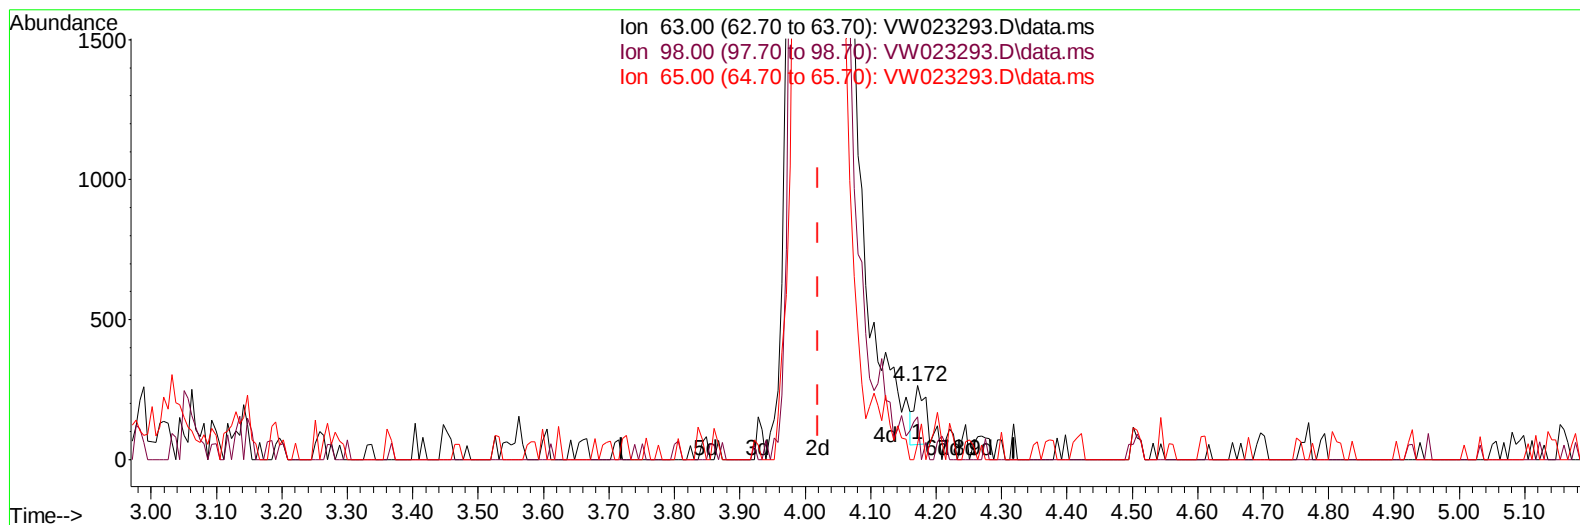

TIC: VW023293.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.172min (+ 0.153) 0.03 ug/L

response 240

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	59.17
65.00	23.30	27.92
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023293.D
 Acq On : 25 May 2022 00:50
 Operator : SY/VA
 Sample : N2995-06
 Misc : 3.47g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 05:59:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

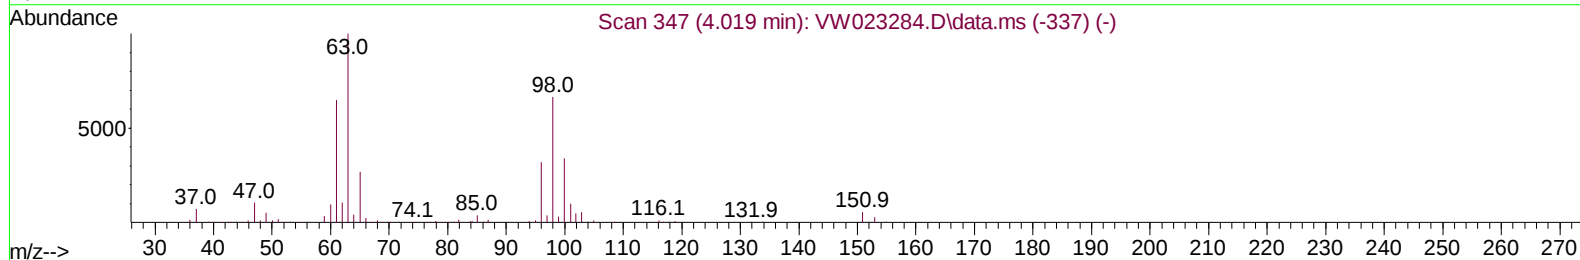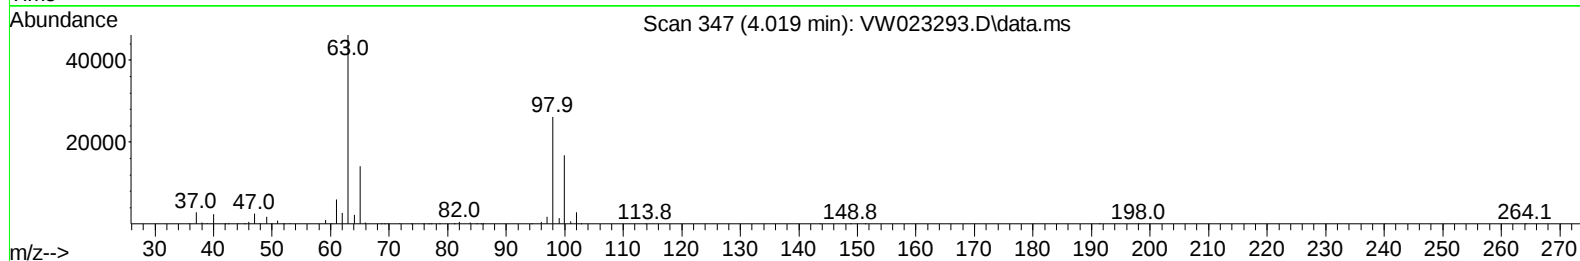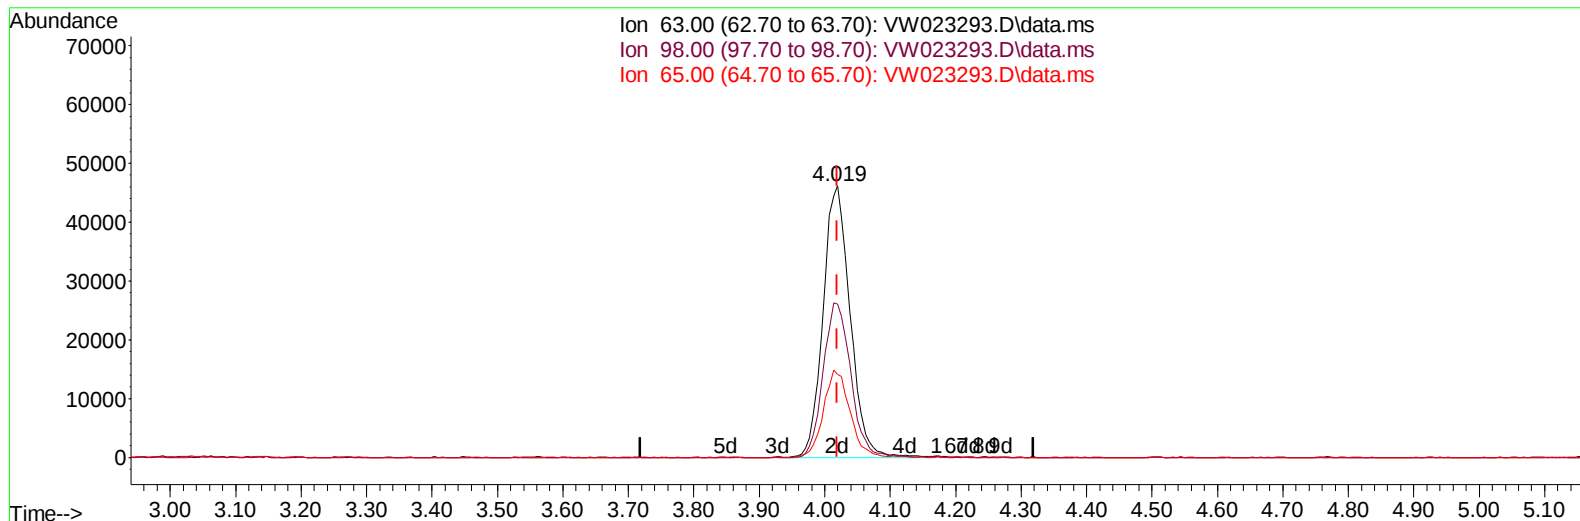

TIC: VW023293.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (+ 0.000) 13.94 ug/L m

response 132252

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.11#
65.00	23.30	0.05#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023293.D
Acq On : 25 May 2022 00:50
Operator : SY/VA
Sample : N2995-06
Misc : 3.47g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGQ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 05:59:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

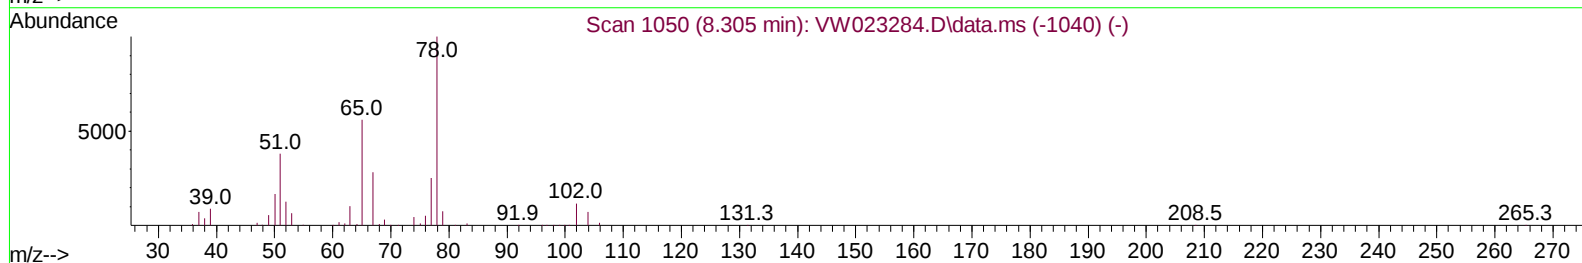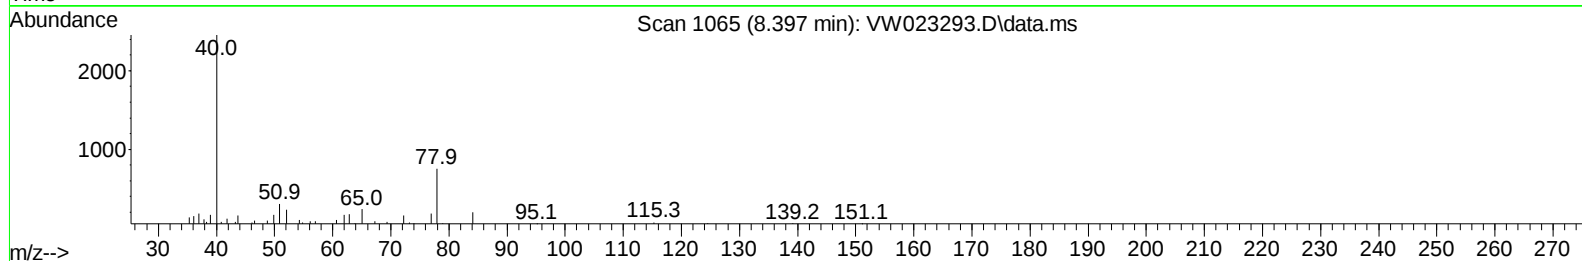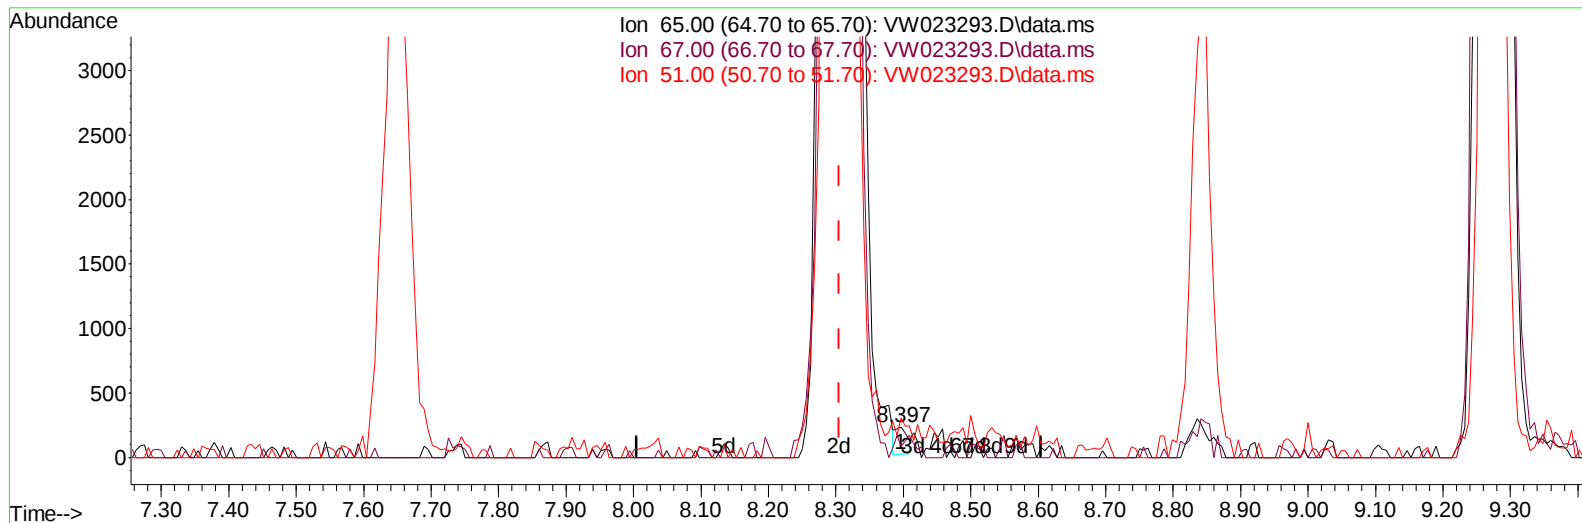

TIC: VW023293.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.397min (+ 0.092) 0.04 ug/L

response 247

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	48.99
51.00	92.30	114.98
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023293.D
 Acq On : 25 May 2022 00:50
 Operator : SY/VA
 Sample : N2995-06
 Misc : 3.47g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 05:59:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

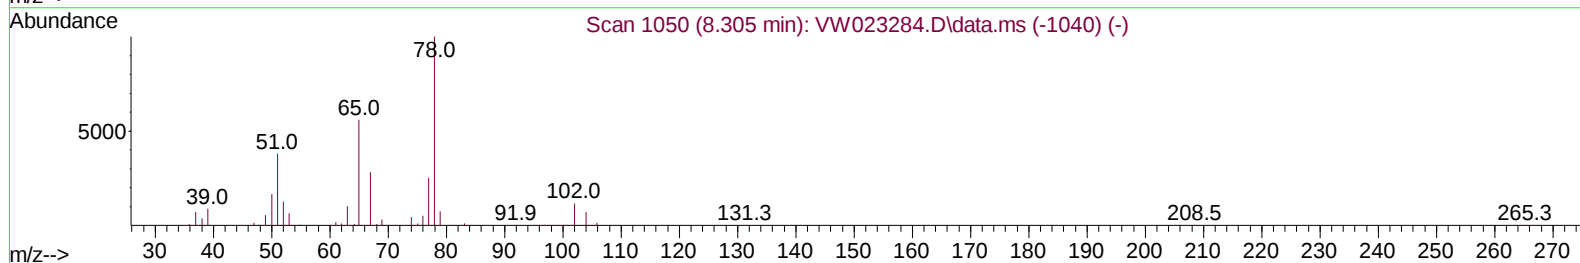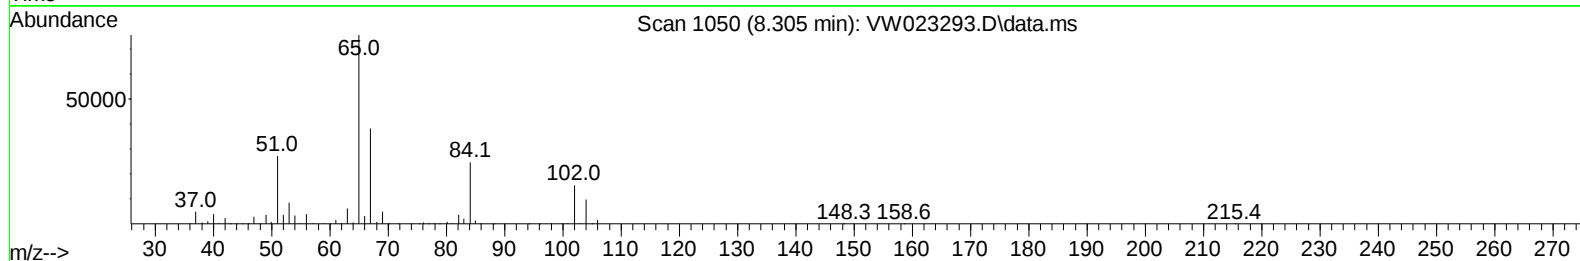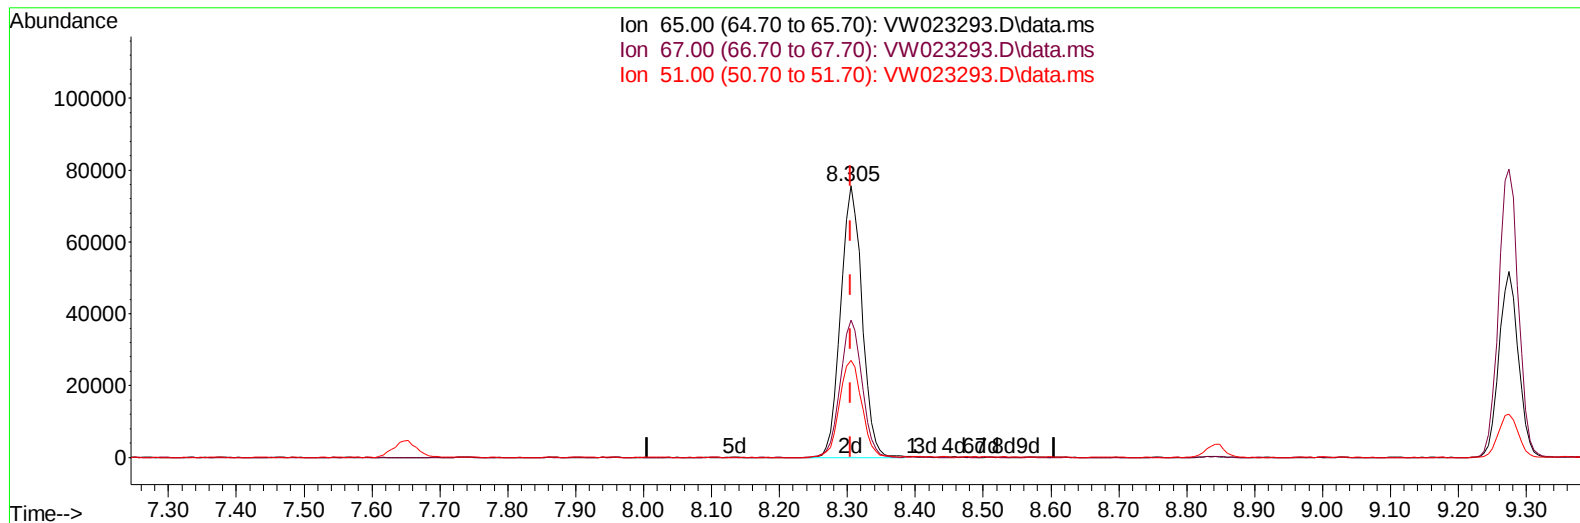

TIC: VW023293.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 28.70 ug/L m

response 164992

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.07#
51.00	92.30	0.17#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023293.D
 Acq On : 25 May 2022 00:50
 Operator : SY/VA
 Sample : N2995-06
 Misc : 3.47g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 05:59:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	357795	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	321316	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	135315	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	134127	18.272	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	73.080%	
7) Chloroethane-d5	2.879	69	85335	17.869	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.480%	
11) 1,1-Dichloroethene-d2	4.019	63	132252m	13.943	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	55.760%	
21) 2-Butanone-d5	7.074	46	85541	61.289	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	122.580%	
24) Chloroform-d	7.647	84	281587	26.862	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	107.440%	
26) 1,2-Dichloroethane-d4	8.305	65	164992m	28.698	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	114.800%	
32) Benzene-d6	8.275	84	482764	26.067	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	104.280%	
36) 1,2-Dichloropropane-d6	9.275	67	161838	31.108	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	124.440%#	
41) Toluene-d8	10.323	98	387052	21.634	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	86.520%	
43) trans-1,3-Dichloroprop...	10.573	79	57351	23.942	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	95.760%	
47) 2-Hexanone-d5	10.921	63	62698	63.131	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	126.260%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	162837	33.581	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	134.320%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	135359	28.616	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	114.480%	
Target Compounds						
13) Acetone	4.129	43	13746	13.155	ug/L	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023293.D
Acq On : 25 May 2022 00:50
Operator : SY/VA
Sample : N2995-06
Misc : 3.47g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGQ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 05:59:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

