




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023294.D
 Acq On : 25 May 2022 01:14
 Operator : SY/VA
 Sample : N2995-07
 Misc : 5.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR0

Manual IntegrationsAPPROVED

Quant Time: May 25 05:59:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

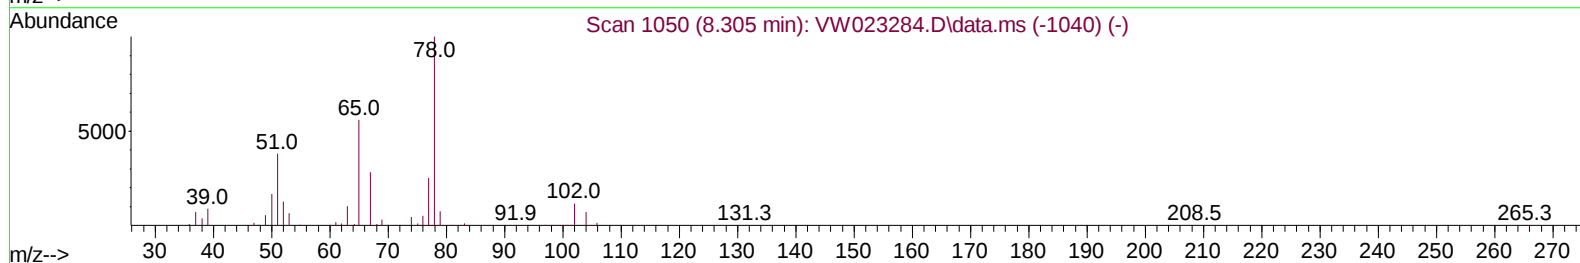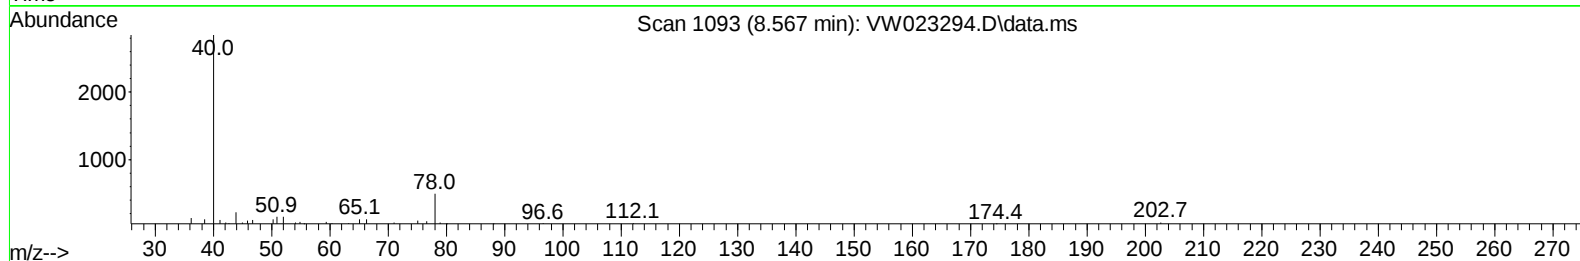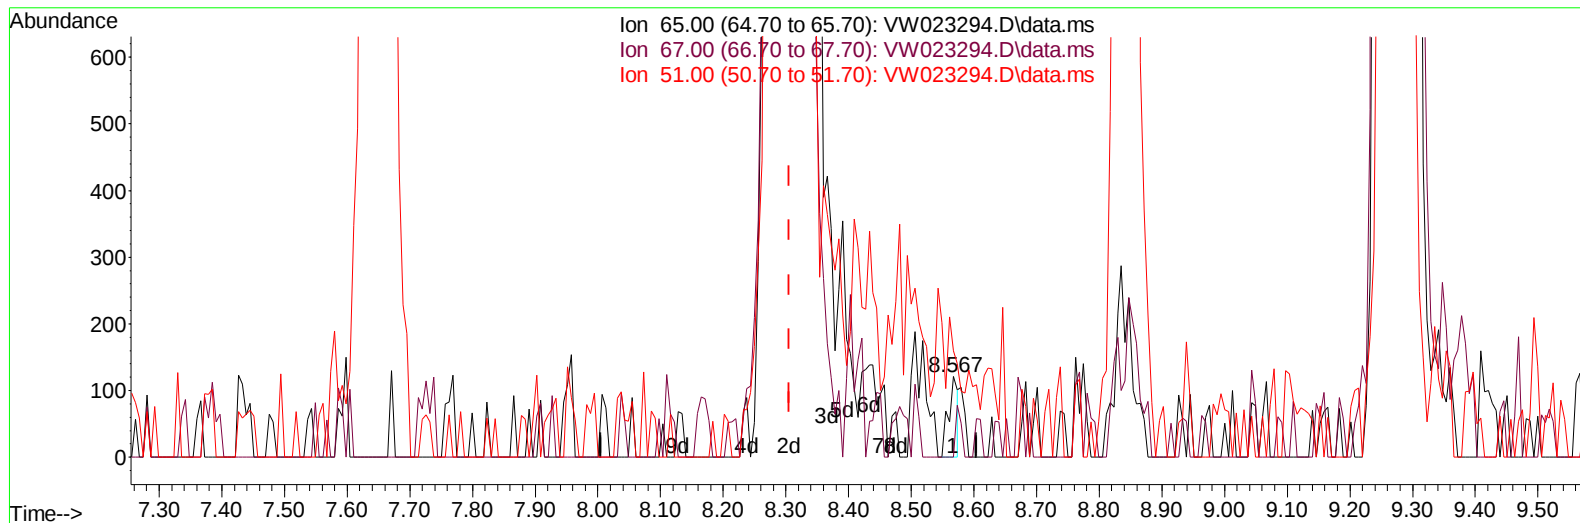

TIC: VW023294.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.567min (+ 0.262) 0.03 ug/L

response 126

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	37.30
51.00	92.30	65.87
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023294.D
 Acq On : 25 May 2022 01:14
 Operator : SY/VA
 Sample : N2995-07
 Misc : 5.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 05:59:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

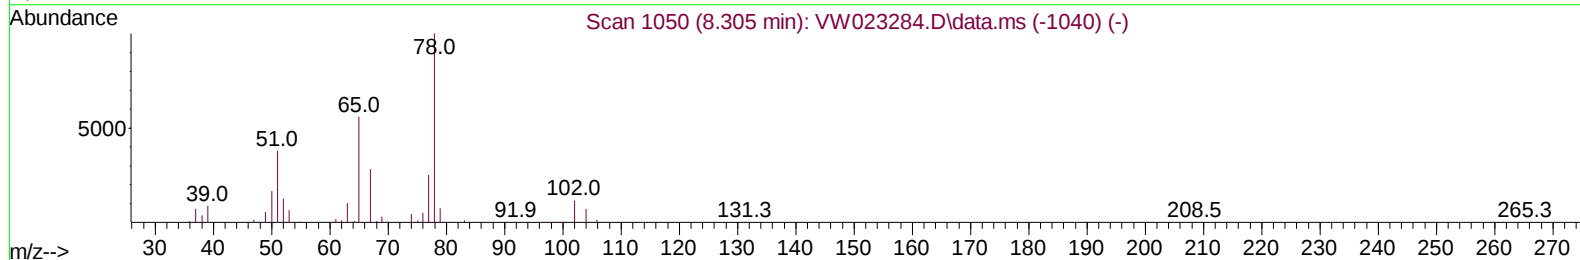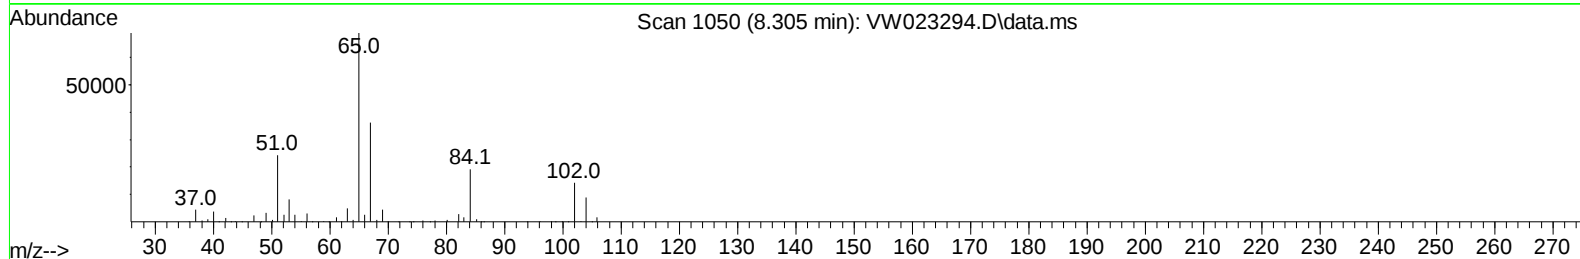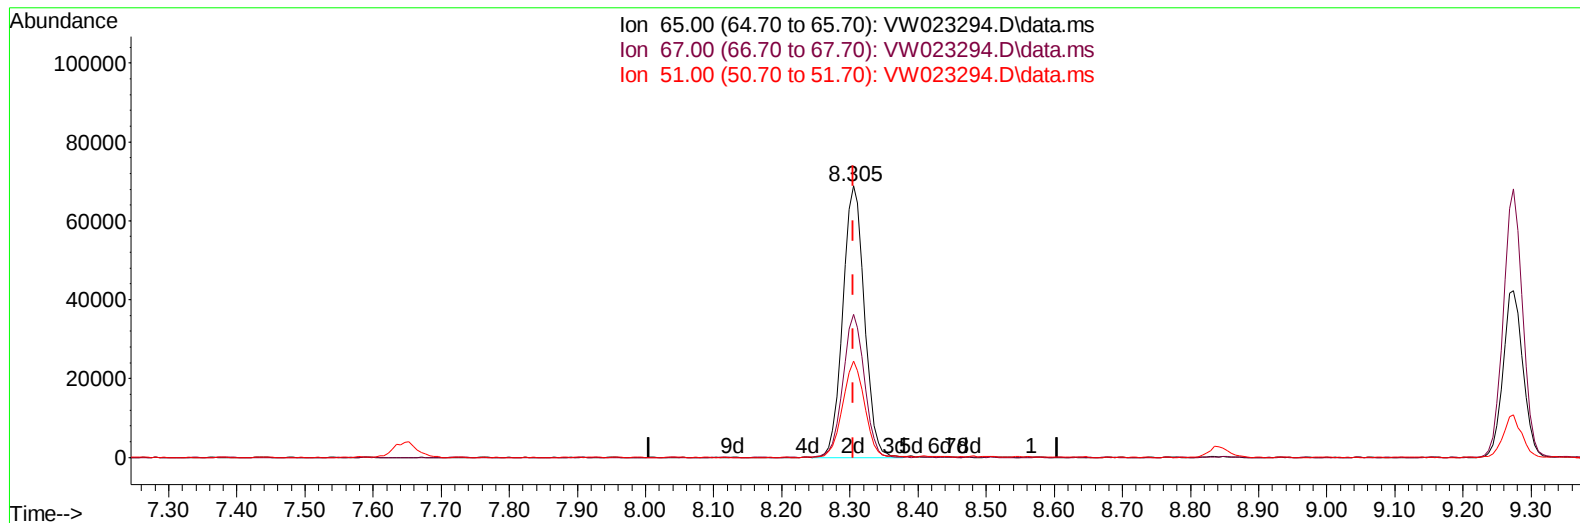

TIC: VW023294.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 34.61 ug/L m

response 151004

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.03#
51.00	92.30	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023294.D
 Acq On : 25 May 2022 01:14
 Operator : SY/VA
 Sample : N2995-07
 Misc : 5.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR0

Manual IntegrationsAPPROVED

Quant Time: May 25 05:59:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		271560	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		244759	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		100237	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		116913	20.984	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.920%	
7) Chloroethane-d5	2.879	69		67873	18.725	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	74.920%	
11) 1,1-Dichloroethene-d2	4.013	63		110100	15.294	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	61.160%	
21) 2-Butanone-d5	7.080	46		104220	98.385	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	196.760%#	
24) Chloroform-d	7.647	84		230471	28.968	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	115.880%	
26) 1,2-Dichloroethane-d4	8.305	65		151004m	34.605	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	138.440%#	
32) Benzene-d6	8.275	84		398251	28.229	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	112.920%	
36) 1,2-Dichloropropane-d6	9.274	67		133352	33.650	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	134.600%#	
41) Toluene-d8	10.323	98		313708	23.019	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	92.080%	
43) trans-1,3-Dichloroprop...	10.579	79		50702	27.787	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	111.160%	
47) 2-Hexanone-d5	10.920	63		80067	105.837	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	211.680%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		168037	45.493	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	181.960%#	
66) 1,2-Dichlorobenzene-d4	13.847	152		104841	29.921	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	119.680%	
Target Compounds							
13) Acetone	4.129	43		11514	14.518	ug/L	Qvalue 74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023294.D
Acq On : 25 May 2022 01:14
Operator : SY/VA
Sample : N2995-07
Misc : 5.79g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGR0

Manual IntegrationsAPPROVED

Quant Time: May 25 05:59:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

