

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023296.D
 Acq On : 25 May 2022 02:02
 Operator : SY/VA
 Sample : N2995-09
 Misc : 3.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR2

Manual IntegrationsAPPROVED

Quant Time: May 25 05:59:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

05/26/2022
 Supervised By :Mahesh
 Dadoda

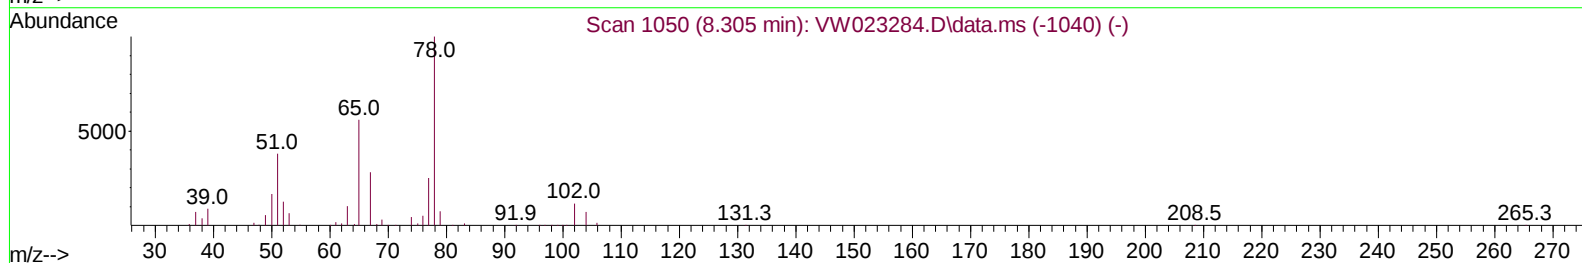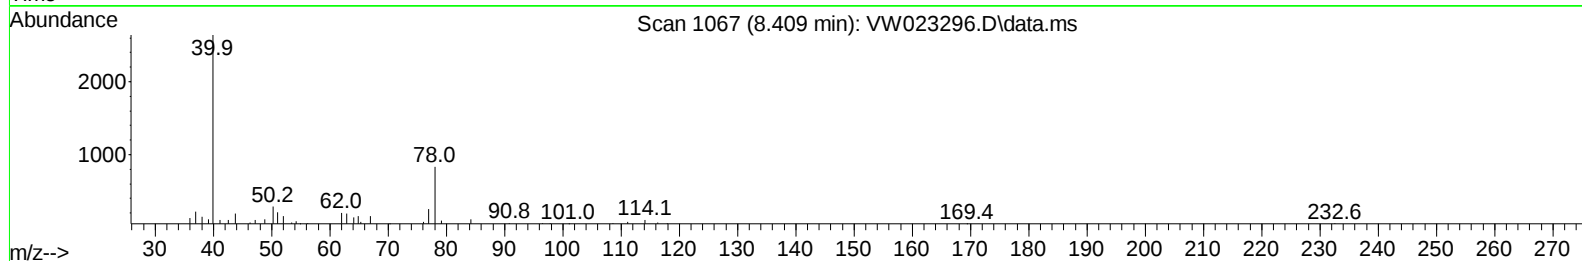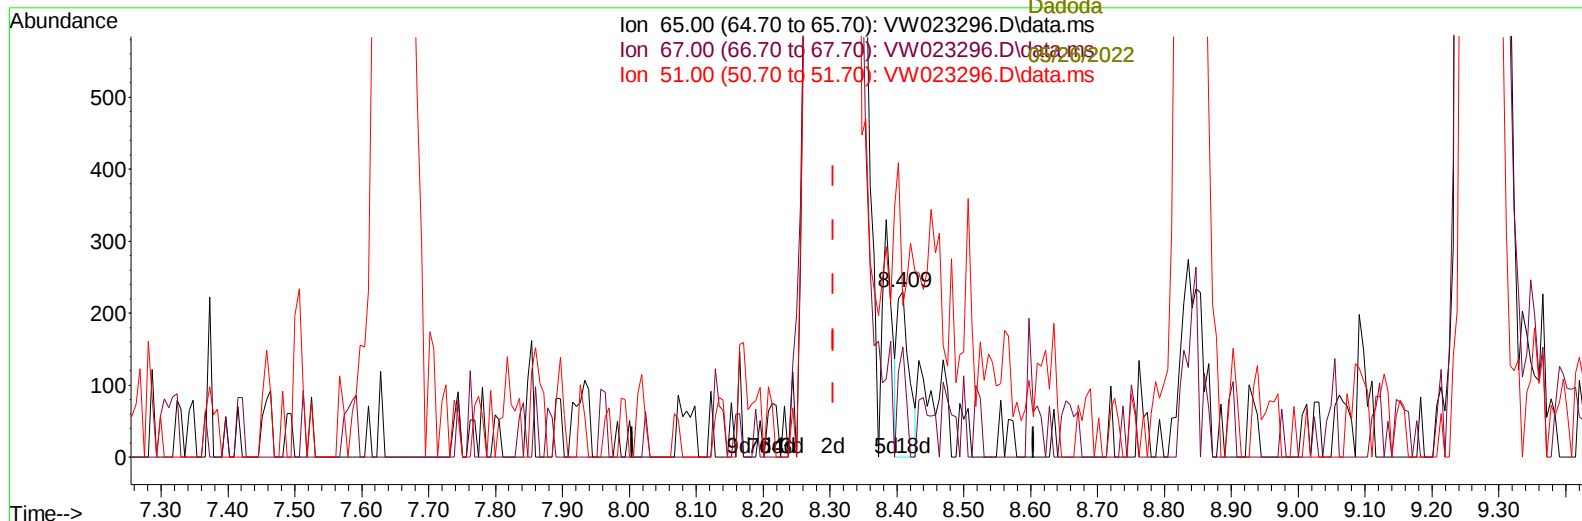

TIC: VW023296.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.409min (+ 0.104) 0.05 ug/L

response 280

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	45.71
51.00	92.30	112.86
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023296.D
 Acq On : 25 May 2022 02:02
 Operator : SY/VA
 Sample : N2995-09
 Misc : 3.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR2




Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

05/26/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: May 25 05:59:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Ion 65.00 (64.70 to 65.70): VW023296.D\data.ms
 Ion 67.00 (66.70 to 67.70): VW023296.D\data.ms
 Ion 51.00 (50.70 to 51.70): VW023296.D\data.ms

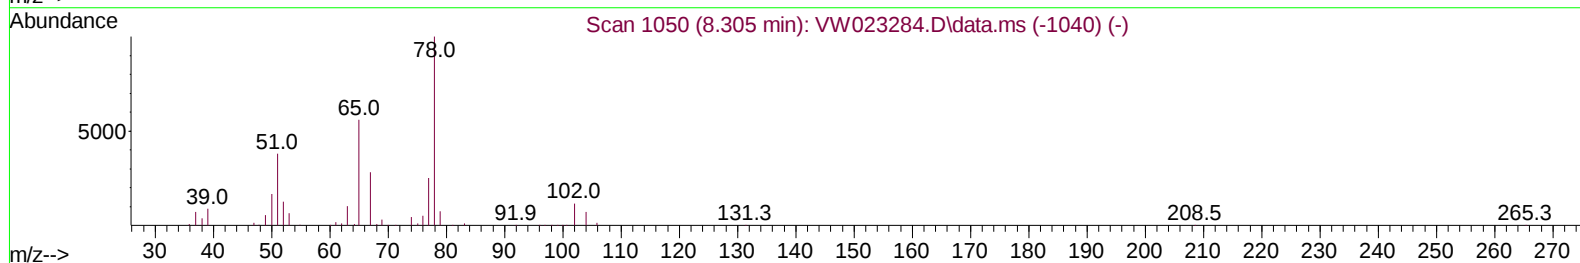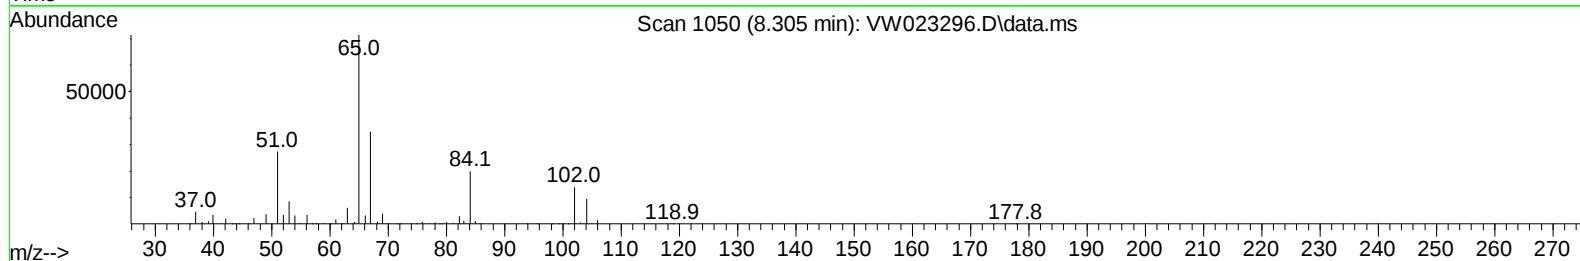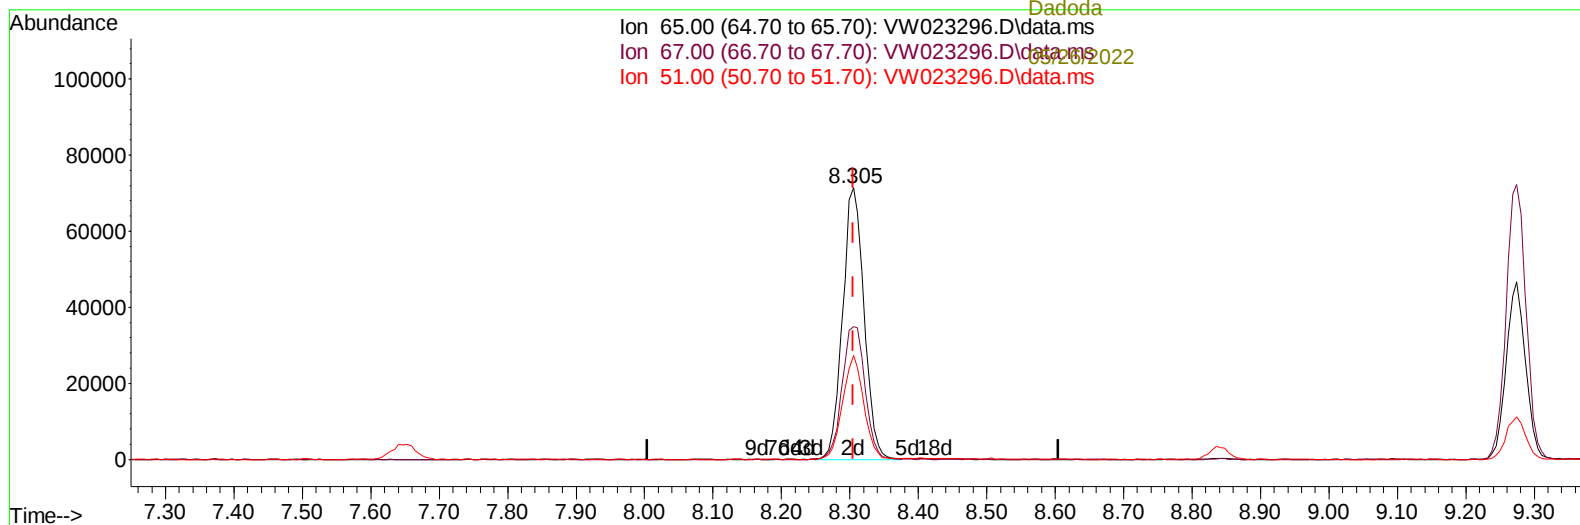

TIC: VW023296.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (0.000) 28.70 ug/L m

response 155535

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.08#
51.00	92.30	0.20#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023296.D
 Acq On : 25 May 2022 02:02
 Operator : SY/VA
 Sample : N2995-09
 Misc : 3.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

05/26/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: May 25 05:59:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----05/26/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	337221	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	308614	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	126419	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	125030	18.072	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	72.280%	
7) Chloroethane-d5	2.879	69	71433	15.870	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.480%	
11) 1,1-Dichloroethene-d2	4.013	63	119459	13.363	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	53.440%	
21) 2-Butanone-d5	7.080	46	90129	68.516	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	137.040%#	
24) Chloroform-d	7.647	84	250731	25.378	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	101.520%	
26) 1,2-Dichloroethane-d4	8.305	65	155535m	28.703	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	114.800%	
32) Benzene-d6	8.275	84	428897	24.111	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	96.440%	
36) 1,2-Dichloropropane-d6	9.274	67	146571	29.333	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	117.320%	
41) Toluene-d8	10.323	98	346845	20.185	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	80.720%	
43) trans-1,3-Dichloroprop...	10.579	79	52895	22.991	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	91.960%	
47) 2-Hexanone-d5	10.920	63	69625	72.992	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	145.980%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	159049	34.150	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	136.600%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	118469	26.808	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	107.240%	
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	32136	32.630	ug/L	97
34) Trichloroethene	9.098	95	3231	0.646	ug/L #	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023296.D
Acq On : 25 May 2022 02:02
Operator : SY/VA
Sample : N2995-09
Misc : 3.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGR2

Manual IntegrationsAPPROVED

Quant Time: May 25 05:59:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

05/26/2022
Supervised By :Mahesh
Dadoda

05/26/2022

