

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023264.D
 Acq On : 24 May 2022 11:58
 Operator : SY/VA
 Sample : N2996-01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGS4

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/26/2022
 Supervised By : Mahesh Dadoda 05/26/2022

Quant Time: May 25 00:50:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 00:48:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	368444	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	372406	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	197294	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	119942	15.867	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.480%		
7) Chloroethane-d5	2.885	69	86019	17.491	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.960%		
11) 1,1-Dichloroethene-d2	4.019	63	126250	12.926	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	51.720%		
21) 2-Butanone-d5	7.074	46	88980	61.910	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	123.820%		
24) Chloroform-d	7.647	84	247682	22.945	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.800%		
26) 1,2-Dichloroethane-d4	8.305	65	148816	25.136	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.560%		
32) Benzene-d6	8.275	84	449010	20.918	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.680%		
36) 1,2-Dichloropropane-d6	9.275	67	140470	23.297	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.200%		
41) Toluene-d8	10.323	98	419085	20.211	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.840%		
43) trans-1,3-Dichloroprop...	10.579	79	61773	22.250	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	89.000%		
47) 2-Hexanone-d5	10.921	63	73078	63.488	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	126.980%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	159354	28.355	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	113.400%		
66) 1,2-Dichlorobenzene-d4	13.853	152	160122	23.217	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.880%		
Target Compounds					Qvalue	
13) Acetone	4.117	43	8421m	7.826	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023264.D
Acq On : 24 May 2022 11:58
Operator : SY/VA
Sample : N2996-01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBGS4

Quant Time: May 25 00:50:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 00:48:22 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

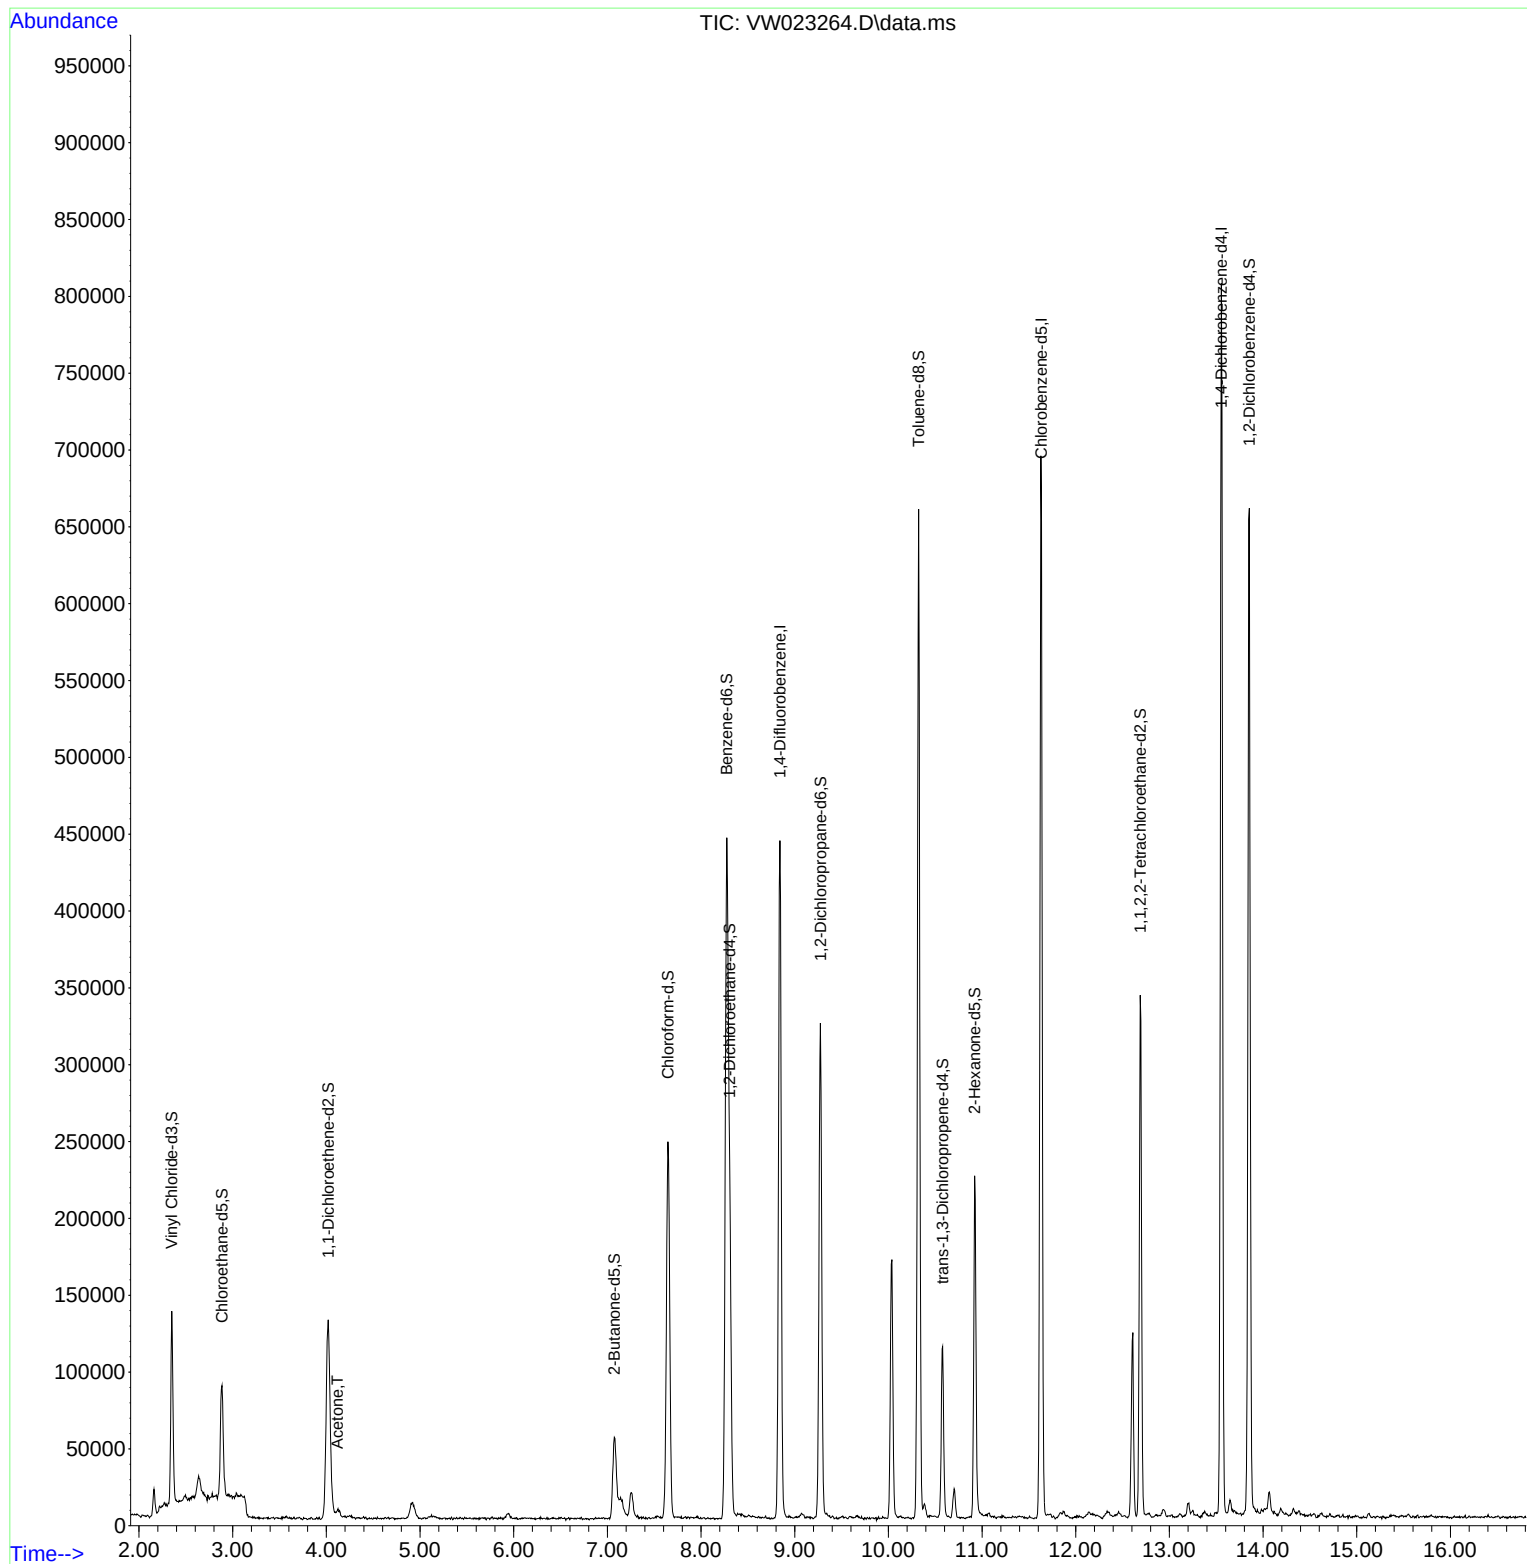

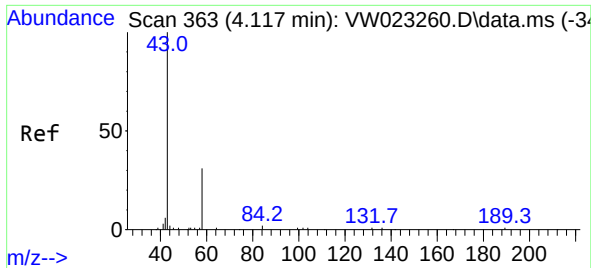

#13

Acetone

Concen: 7.826 ug/L m

RT: 4.117 min Scan# 30

Delta R.T. -0.000 min

Lab File: VW023264.D

Acq: 24 May 2022 11:58

Instrument :

MSVOA_W

ClientSampleId :

GBGS4

Tgt Ion: 43 Resp: 842

Ion Ratio Lower Upper

43 100

58 25.0 0.0 64.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022

Supervised By :Mahesh Dadoda 05/26/2022

