

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023276.D
 Acq On : 24 May 2022 16:47
 Operator : SY/VA
 Sample : N2996-18
 Misc : 4.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGT9

Quant Time: May 25 00:52:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 00:48:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	331671	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	344685	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	171729	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	108504	15.945	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.800%
7) Chloroethane-d5	2.886	69	82314	18.594	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.360%
11) 1,1-Dichloroethene-d2	4.013	63	109403	12.443	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.760%
21) 2-Butanone-d5	7.074	46	83533	64.564	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	129.120%
24) Chloroform-d	7.647	84	227978	23.461	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.840%
26) 1,2-Dichloroethane-d4	8.305	65	140240	26.314	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.240%
32) Benzene-d6	8.275	84	406490	20.460	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.840%
36) 1,2-Dichloropropane-d6	9.275	67	129964	23.288	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.160%
41) Toluene-d8	10.323	98	373697	19.471	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.880%
43) trans-1,3-Dichloroprop...	10.579	79	56441	21.965	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.840%
47) 2-Hexanone-d5	10.921	63	71013	66.656	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	133.320%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	147020	28.264	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	145410	24.223	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.880%
Target Compounds					Qvalue	
13) Acetone	4.123	43	10956	11.311	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023276.D
Acq On : 24 May 2022 16:47
Operator : SY/VA
Sample : N2996-18
Misc : 4.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGT9

Quant Time: May 25 00:52:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 00:48:22 2022
Response via : Initial Calibration

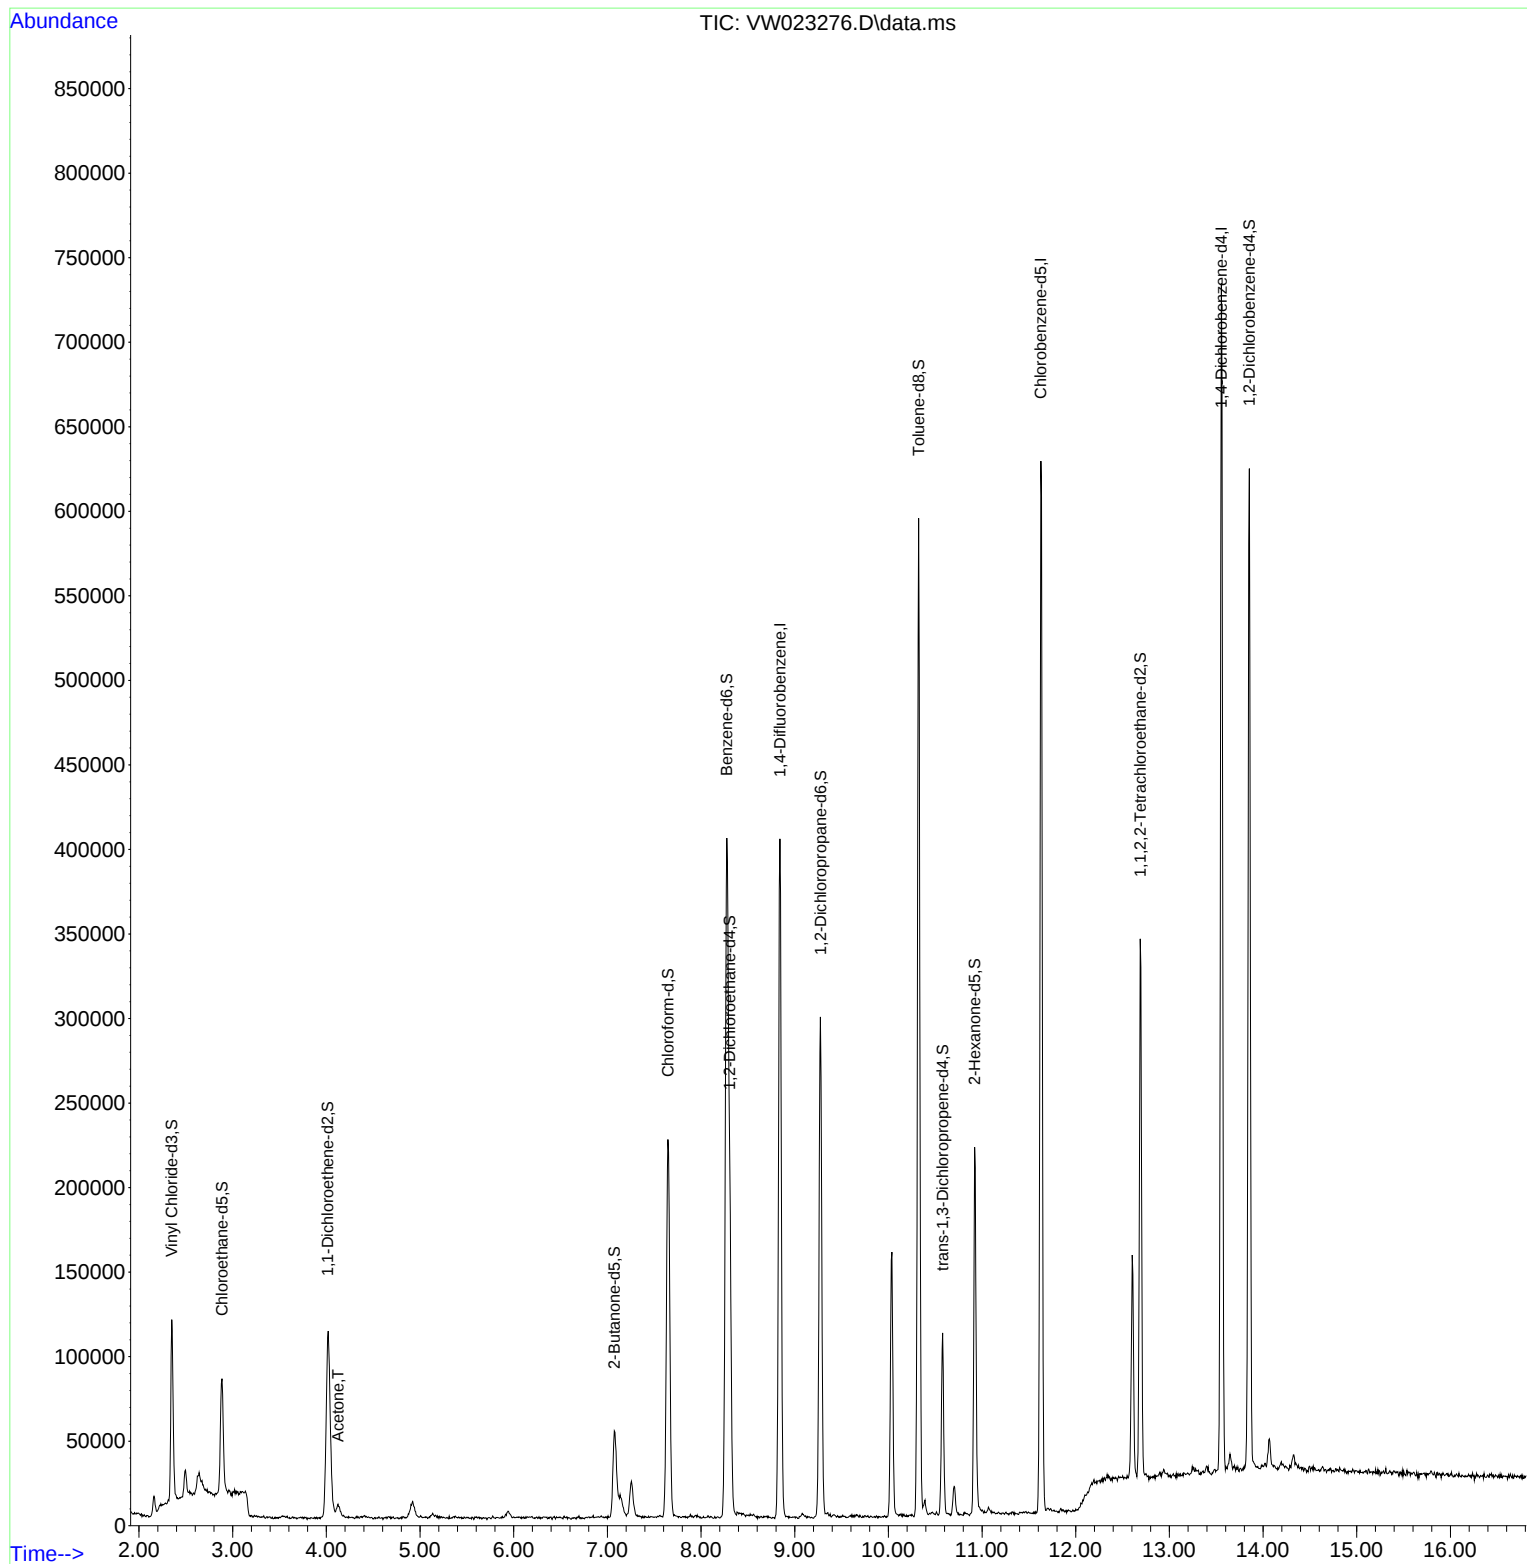

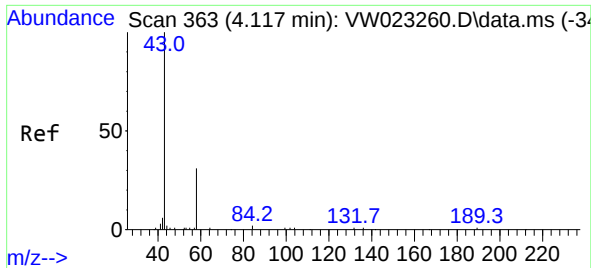

#13
Acetone
Concen: 11.311 ug/L
RT: 4.123 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW023276.D
Acq: 24 May 2022 16:47

Instrument :
MSVOA_W
ClientSampleId :
GBGT9

Tgt Ion: 43 Resp: 10956
Ion Ratio Lower Upper
43 100
58 25.5 0.0 64.0

