

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
 Data File : VW023293.D
 Acq On : 25 May 2022 00:50
 Operator : SY/VA
 Sample : N2995-06
 Misc : 3.47g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ9

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 25 05:59:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 25 04:05:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	357795	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	321316	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	135315	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	134127	18.272	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.080%
7) Chloroethane-d5	2.879	69	85335	17.869	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.480%
11) 1,1-Dichloroethene-d2	4.019	63	132252m	13.943	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.760%
21) 2-Butanone-d5	7.074	46	85541	61.289	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.580%
24) Chloroform-d	7.647	84	281587	26.862	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	107.440%
26) 1,2-Dichloroethane-d4	8.305	65	164992m	28.698	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	114.800%
32) Benzene-d6	8.275	84	482764	26.067	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.280%
36) 1,2-Dichloropropane-d6	9.275	67	161838	31.108	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	124.440%#
41) Toluene-d8	10.323	98	387052	21.634	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.520%
43) trans-1,3-Dichloroprop...	10.573	79	57351	23.942	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.760%
47) 2-Hexanone-d5	10.921	63	62698	63.131	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.260%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	162837	33.581	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	134.320%#
66) 1,2-Dichlorobenzene-d4	13.853	152	135359	28.616	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	114.480%
Target Compounds					Qvalue	
13) Acetone	4.129	43	13746	13.155	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052422\
Data File : VW023293.D
Acq On : 25 May 2022 00:50
Operator : SY/VA
Sample : N2995-06
Misc : 3.47g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBGQ9

Quant Time: May 25 05:59:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 25 04:05:49 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

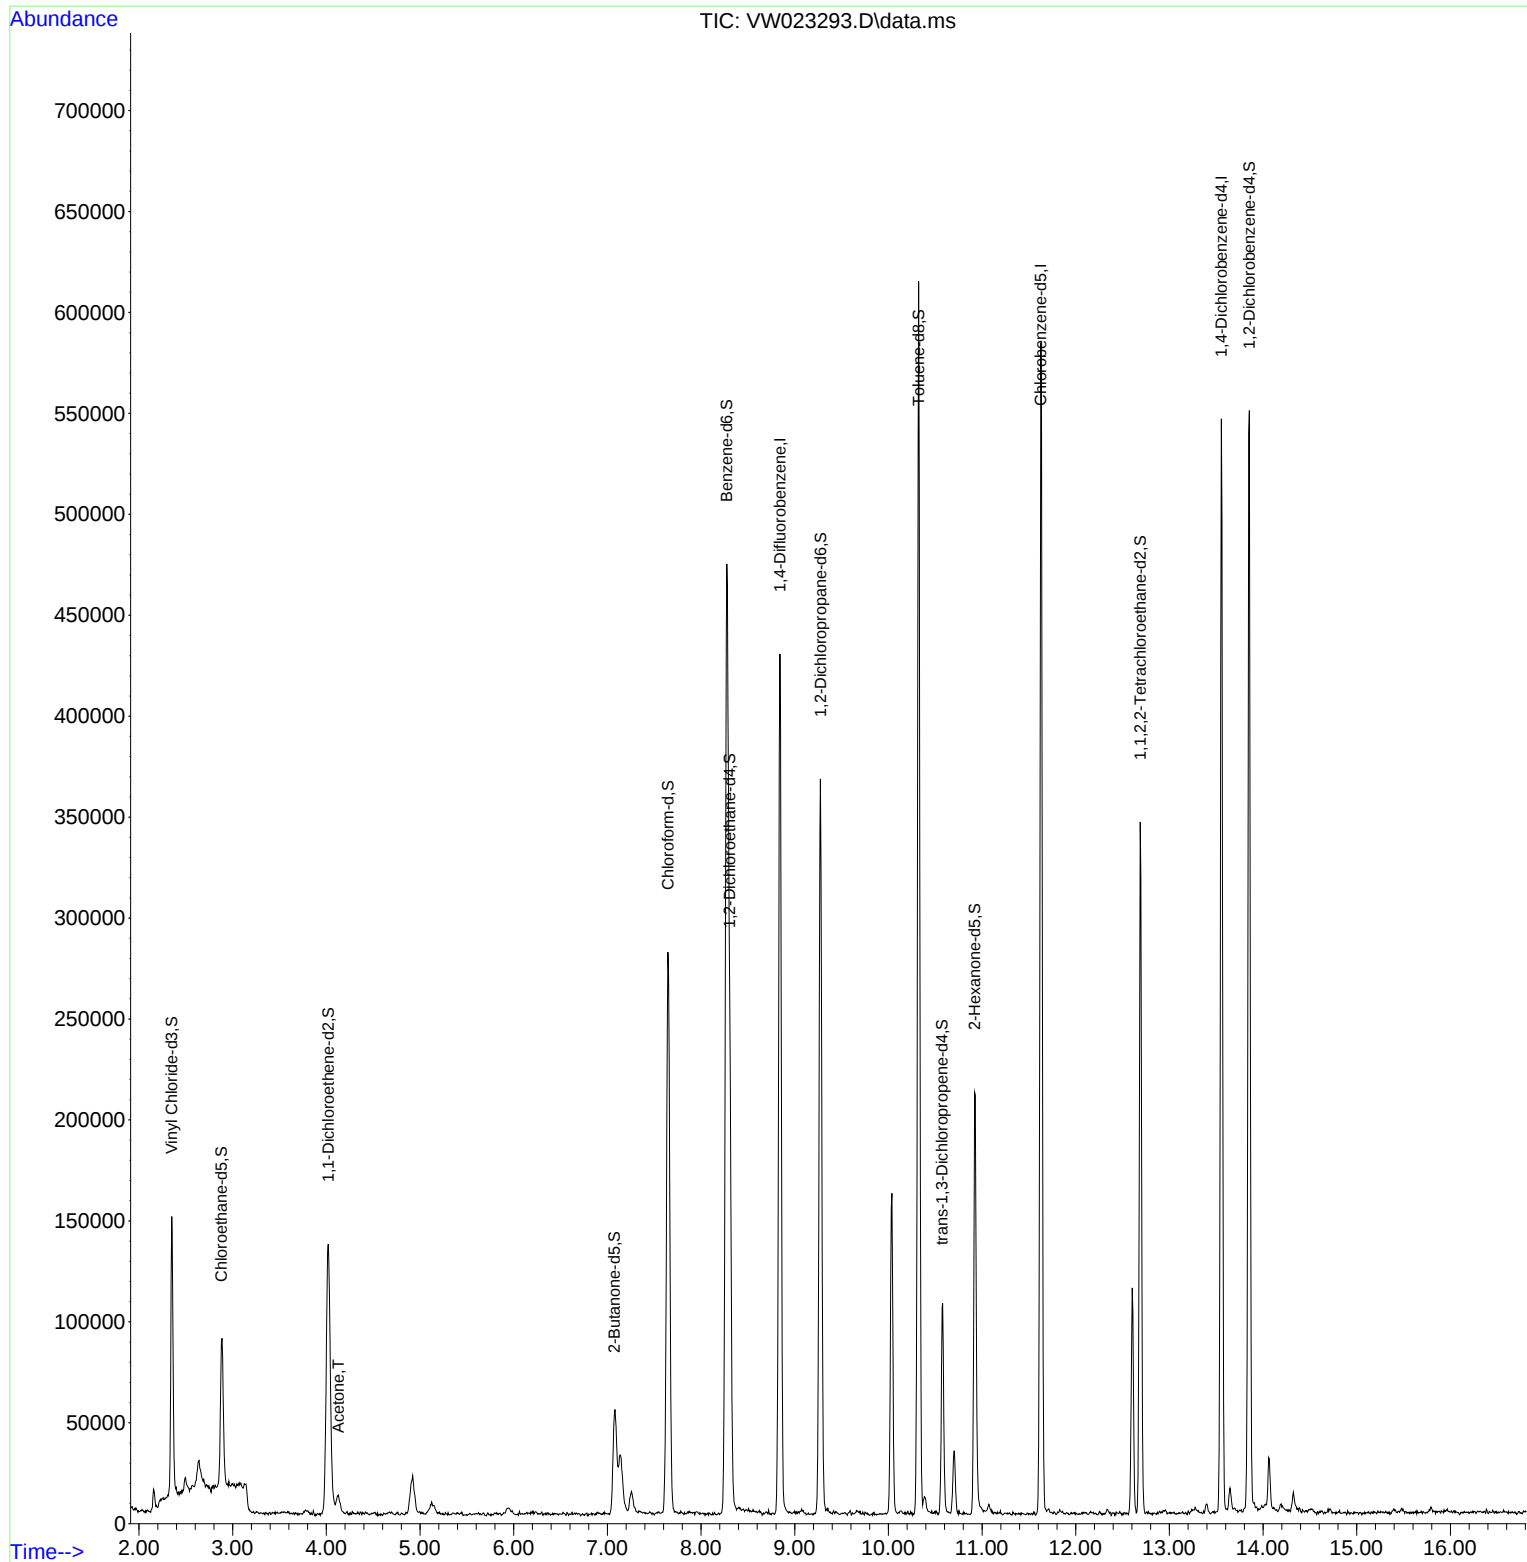

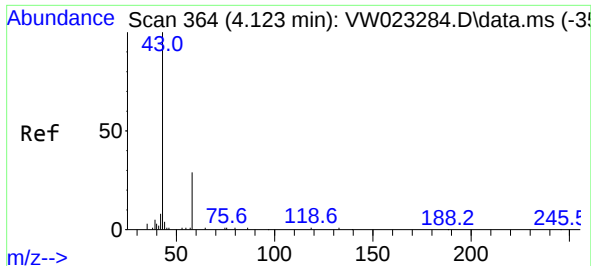

#13
 Acetone
 Concen: 13.155 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW023293.D
 Acq: 25 May 2022 00:50

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ9

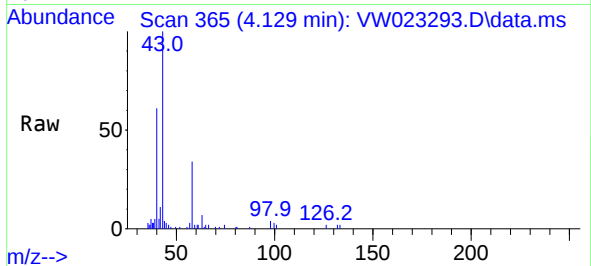

Tgt Ion: 43 Resp: 13740
 Ion Ratio Lower Upper
 43 100
 58 37.0 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

