




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052423\
 Data File : VW026028.D
 Acq On : 24 May 2023 13:30
 Operator : SY/MD
 Sample : 02917-02
 Misc : 5.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11G3

Manual IntegrationsAPPROVED

Quant Time: May 25 00:24:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 25 00:24:12 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

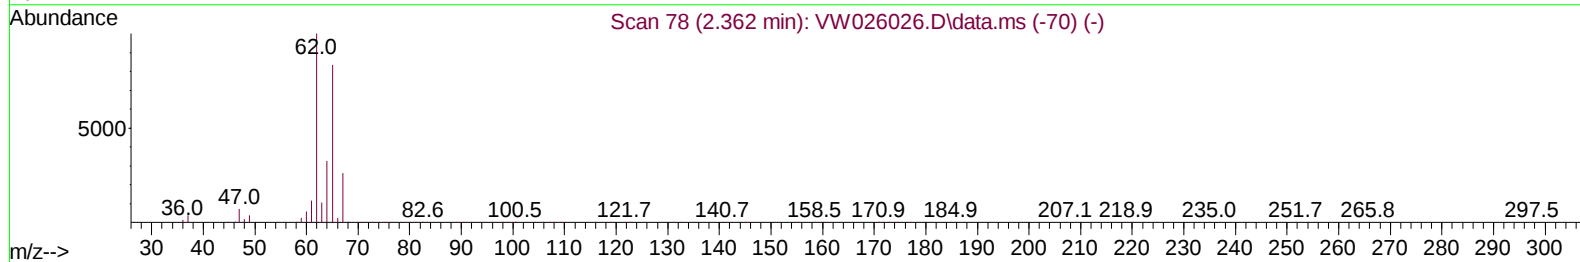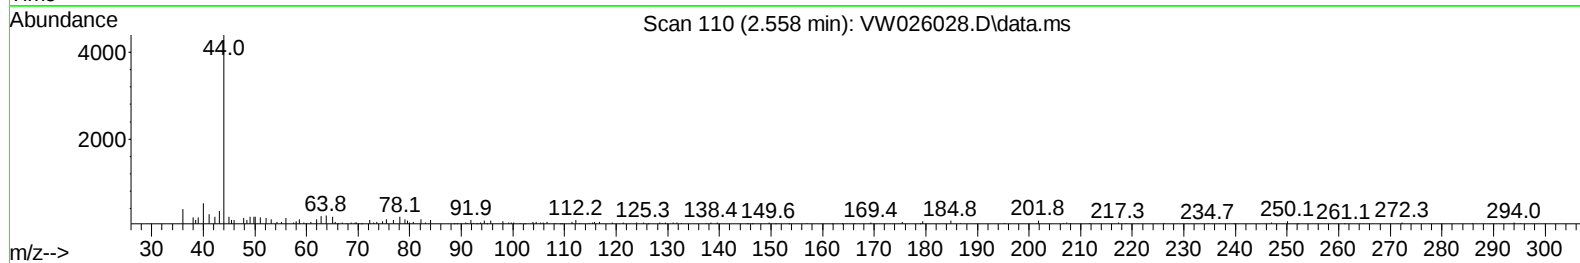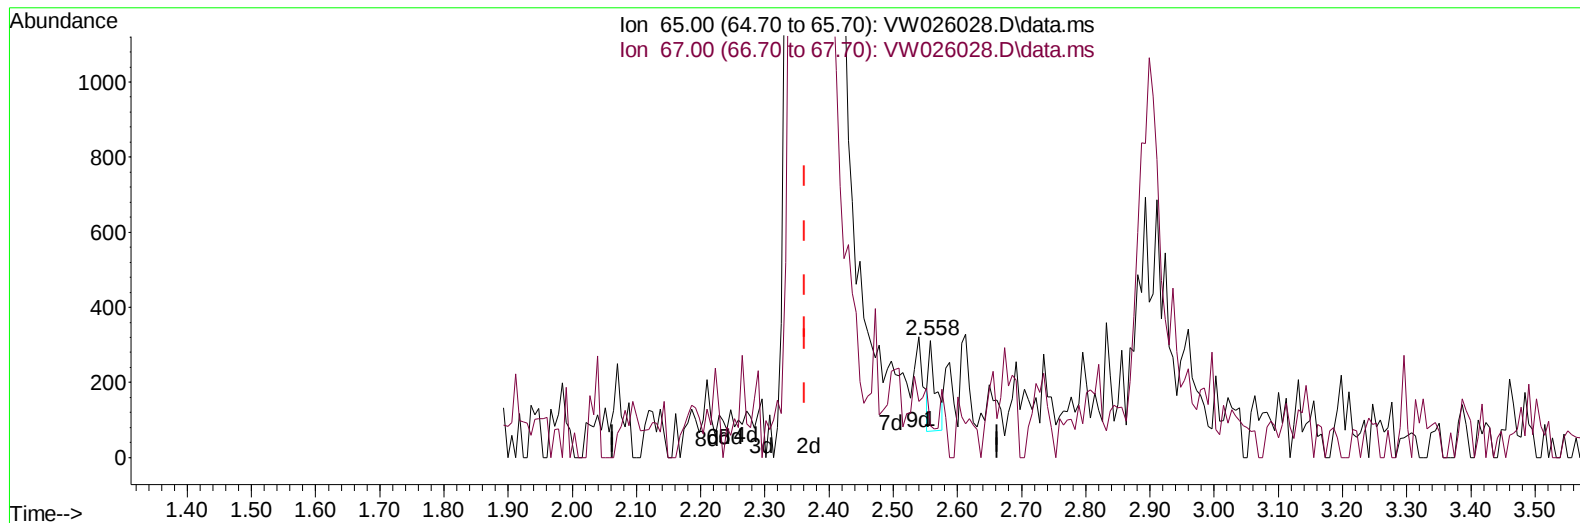

TIC: VW026028.D\data.ms

(4) Vinyl Chloride-d3 (S)

2.558min (+ 0.195) 0.03 ug/L

response 190

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.00	38.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052423\
 Data File : VW026028.D
 Acq On : 24 May 2023 13:30
 Operator : SY/MD
 Sample : 02917-02
 Misc : 5.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11G3

Manual IntegrationsAPPROVED

Quant Time: May 25 00:24:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 25 00:24:12 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/25/2023
 Supervised By :Mahesh Dadoda 05/25/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		412346	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		298142	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		51636	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		90102m	15.420	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	61.680%	
7) Chloroethane-d5	2.893	69		89972	20.769	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.080%	
11) 1,1-Dichloroethene-d2	4.021	65		47113	16.102	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	64.400%	
21) 2-Butanone-d5	7.075	46		146500	75.840	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	151.680%#	
24) Chloroform-d	7.648	84		315073	26.499	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	106.000%	
26) 1,2-Dichloroethane-d4	8.301	65		211942	31.522	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	126.080%	
32) Benzene-d6	8.270	84		543998	27.924	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	111.680%	
36) 1,2-Dichloropropane-d6	9.270	67		218695	35.086	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	140.360%#	
41) Toluene-d8	10.318	98		385440	22.188	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	88.760%	
43) trans-1,3-Dichloroprop...	10.575	79		64537	25.543	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	102.160%	
47) 2-Hexanone-d5	10.922	63		88819	83.566	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	167.140%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		183695	38.666	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	154.680%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		53655	28.504	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	114.000%	
Target Compounds							
						Qvalue	
13) Acetone	4.124	43		22642	13.219	ug/L	98
16) Methylene chloride	4.917	84		58426	6.871	ug/L	88
20) cis-1,2-Dichloroethene	7.173	96		7412	1.148	ug/L	88
34) Trichloroethene	9.087	95		15913	3.006	ug/L	93
46) Tetrachloroethene	10.861	164		2270032	609.611	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052423\
Data File : VW026028.D
Acq On : 24 May 2023 13:30
Operator : SY/MD
Sample : 02917-02
Misc : 5.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C11G3

Manual IntegrationsAPPROVED

Quant Time: May 25 00:24:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 25 00:24:12 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/25/2023
Supervised By :Mahesh Dadoda 05/25/2023

