




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052623\
 Data File : VW026062.D
 Acq On : 26 May 2023 12:45
 Operator : SY/MD
 Sample : 02950-16
 Misc : 5.17g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW992

Manual IntegrationsAPPROVED

Quant Time: May 26 23:17:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 26 23:14:25 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/29/2023
 Supervised By :Mahesh Dadoda 05/29/2023

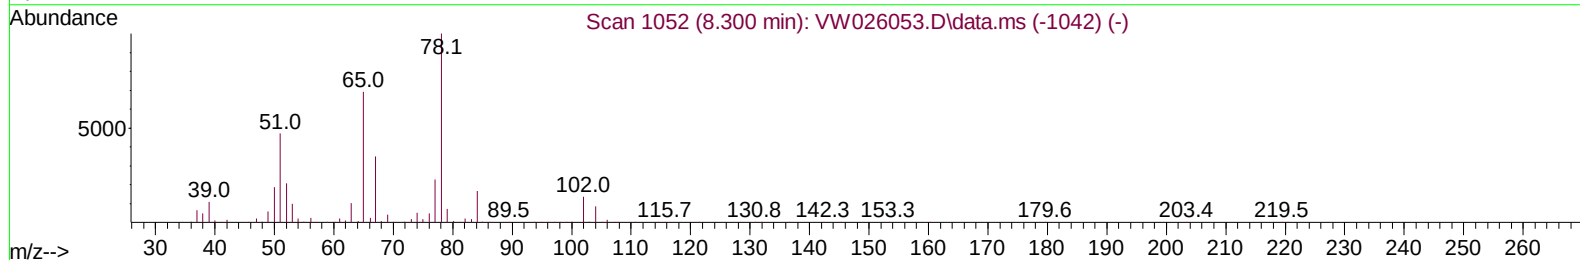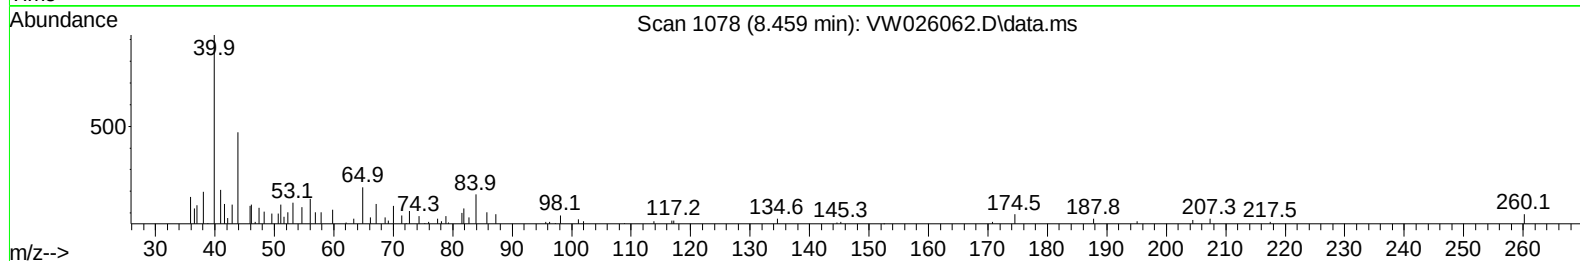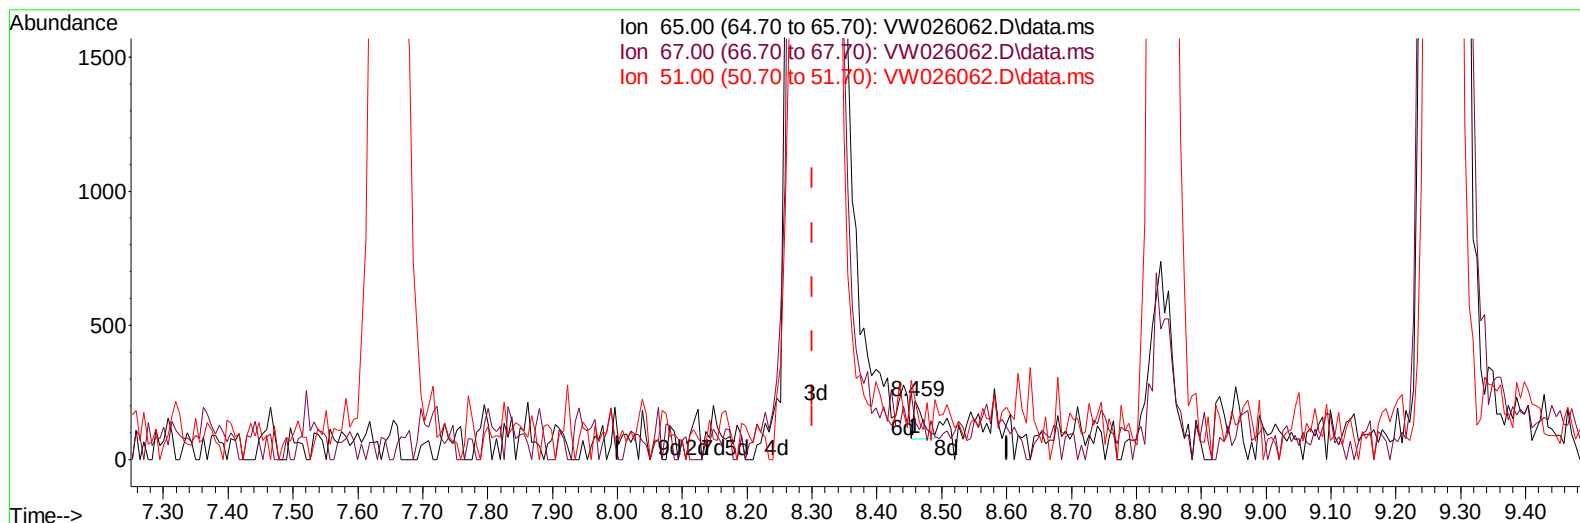

TIC: VW026062.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.459min (+ 0.159) 0.01 ug/L

response 138

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	43.48
51.00	112.30	86.23
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052623\
 Data File : VW026062.D
 Acq On : 26 May 2023 12:45
 Operator : SY/MD
 Sample : 02950-16
 Misc : 5.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW992

Manual IntegrationsAPPROVED

Quant Time: May 26 23:17:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 26 23:14:25 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/29/2023
 Supervised By :Mahesh Dadoda 05/29/2023

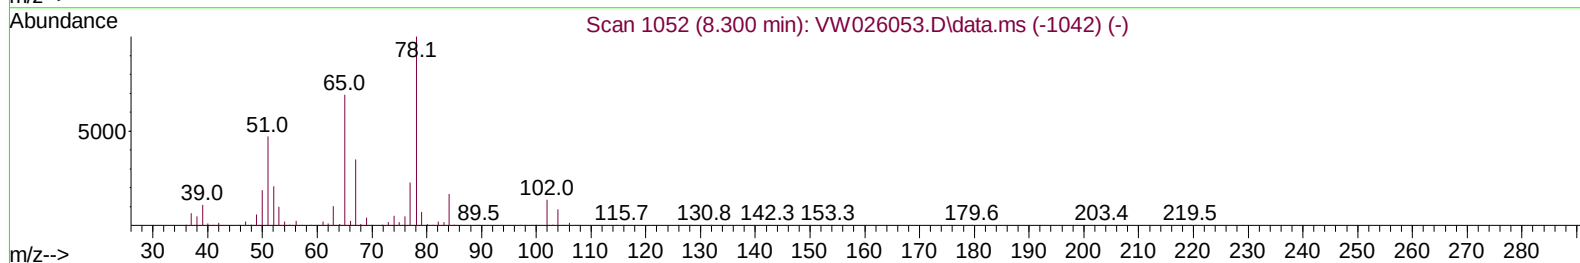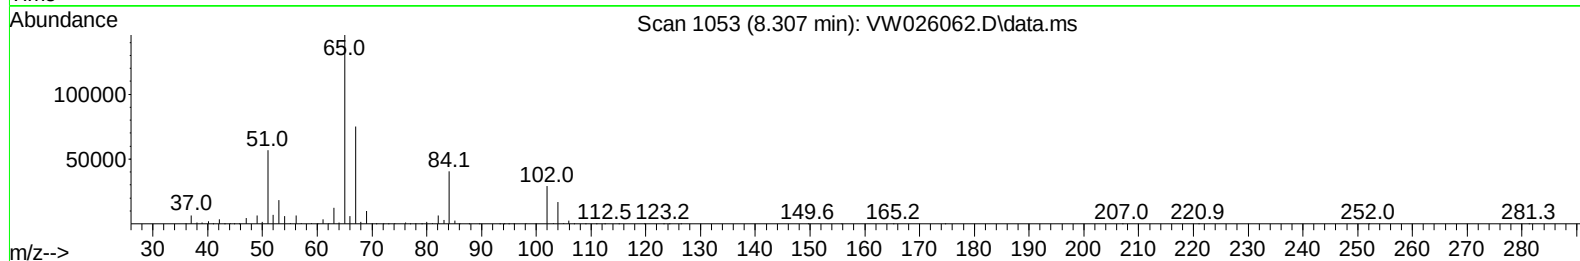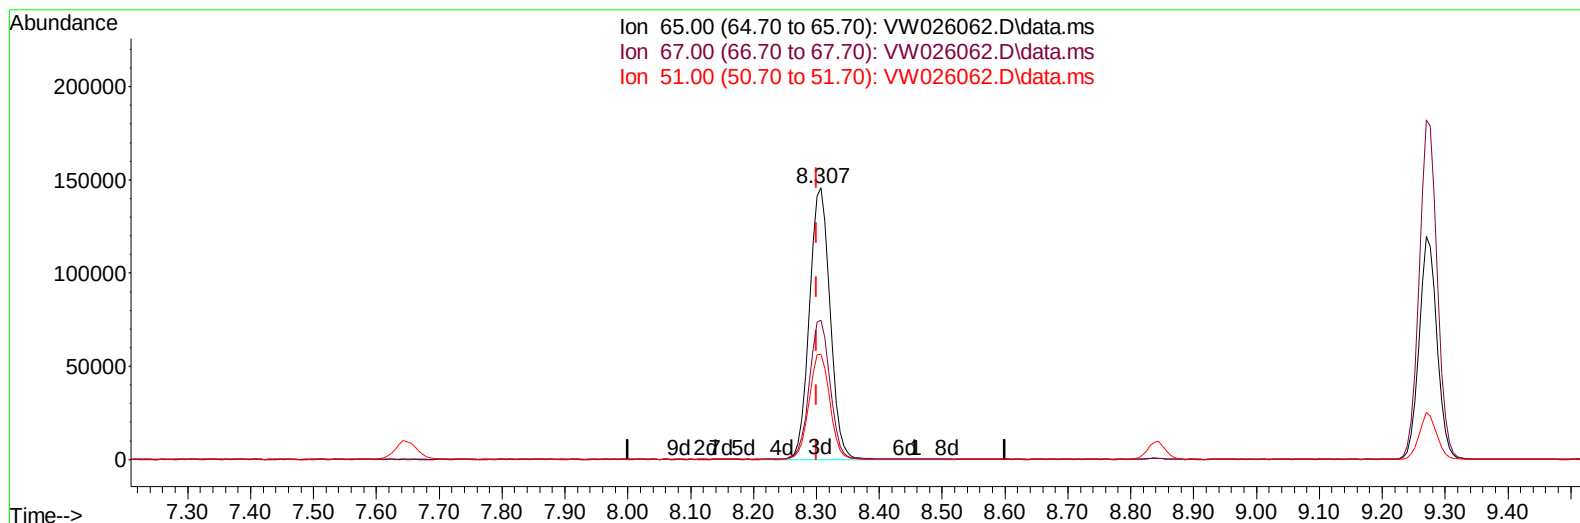

TIC: VW026062.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.007) 24.67 ug/L m

response 333126

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.02#
51.00	112.30	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052623\
 Data File : VW026062.D
 Acq On : 26 May 2023 12:45
 Operator : SY/MD
 Sample : 02950-16
 Misc : 5.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW992

Manual IntegrationsAPPROVED

Quant Time: May 26 23:17:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 26 23:14:25 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/29/2023
 Supervised By :Mahesh Dadoda 05/29/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		828121	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		628782	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		208206	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		221797	18.900	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	75.600%	
7) Chloroethane-d5	2.899	69		205633	23.636	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	94.560%	
11) 1,1-Dichloroethene-d2	4.021	65		110052	18.729	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	74.920%	
21) 2-Butanone-d5	7.075	46		222219	57.281	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	114.560%	
24) Chloroform-d	7.648	84		549919	23.029	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	92.120%	
26) 1,2-Dichloroethane-d4	8.307	65		333126m	24.671	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	98.680%	
32) Benzene-d6	8.276	84		1032359	25.127	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	100.520%	
36) 1,2-Dichloropropane-d6	9.270	67		362428	27.570	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	110.280%	
41) Toluene-d8	10.325	98		784777	21.420	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	85.680%	
43) trans-1,3-Dichloroprop...	10.575	79		112601	21.131	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	84.520%	
47) 2-Hexanone-d5	10.922	63		140111	62.505	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	125.020%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		275095	27.456	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	109.840%	
66) 1,2-Dichlorobenzene-d4	13.849	152		203480	26.809	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	107.240%	
Target Compounds							
						Qvalue	
13) Acetone	4.125	43		48484	14.094	ug/L	78
14) Carbon disulfide	4.381	76		32023	0.855	ug/L	96
16) Methylene chloride	4.917	84		69856	4.090	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052623\
Data File : VW026062.D
Acq On : 26 May 2023 12:45
Operator : SY/MD
Sample : 02950-16
Misc : 5.17g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW992

Manual IntegrationsAPPROVED

Quant Time: May 26 23:17:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 26 23:14:25 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/29/2023
Supervised By :Mahesh Dadoda 05/29/2023

