

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052824\
 Data File : VW028840.D
 Acq On : 28 May 2024 18:42
 Operator : SY/MD
 Sample : P2591-05
 Misc : 5.15g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH5S8

Quant Time: May 29 01:00:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 29 00:53:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	402694	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	318114	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	93588	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	91967	12.027	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	48.120%		
7) Chloroethane-d5	2.899	69	89143	15.225	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.880%		
11) 1,1-Dichloroethene-d2	4.021	65	41714	13.057	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	52.240%		
21) 2-Butanone-d5	7.075	46	74805	37.496	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	75.000%		
24) Chloroform-d	7.648	84	240709	19.130	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	76.520%		
26) 1,2-Dichloroethane-d4	8.307	65	141243	19.607	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	78.440%		
32) Benzene-d6	8.276	84	408930	19.267	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	77.080%		
36) 1,2-Dichloropropane-d6	9.270	67	152673	23.905	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.640%		
41) Toluene-d8	10.319	98	319187	16.982	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	67.920%		
43) trans-1,3-Dichloroprop...	10.575	79	43917	17.093	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	68.360%		
47) 2-Hexanone-d5	10.922	63	47089	42.749	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	85.500%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	125334	23.403	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.600%		
66) 1,2-Dichlorobenzene-d4	13.849	152	77135	21.624	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	86.480%		
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	33951	5.451	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052824\
Data File : VW028840.D
Acq On : 28 May 2024 18:42
Operator : SY/MD
Sample : P2591-05
Misc : 5.15g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH5S8

Quant Time: May 29 01:00:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 29 00:53:59 2024
Response via : Initial Calibration

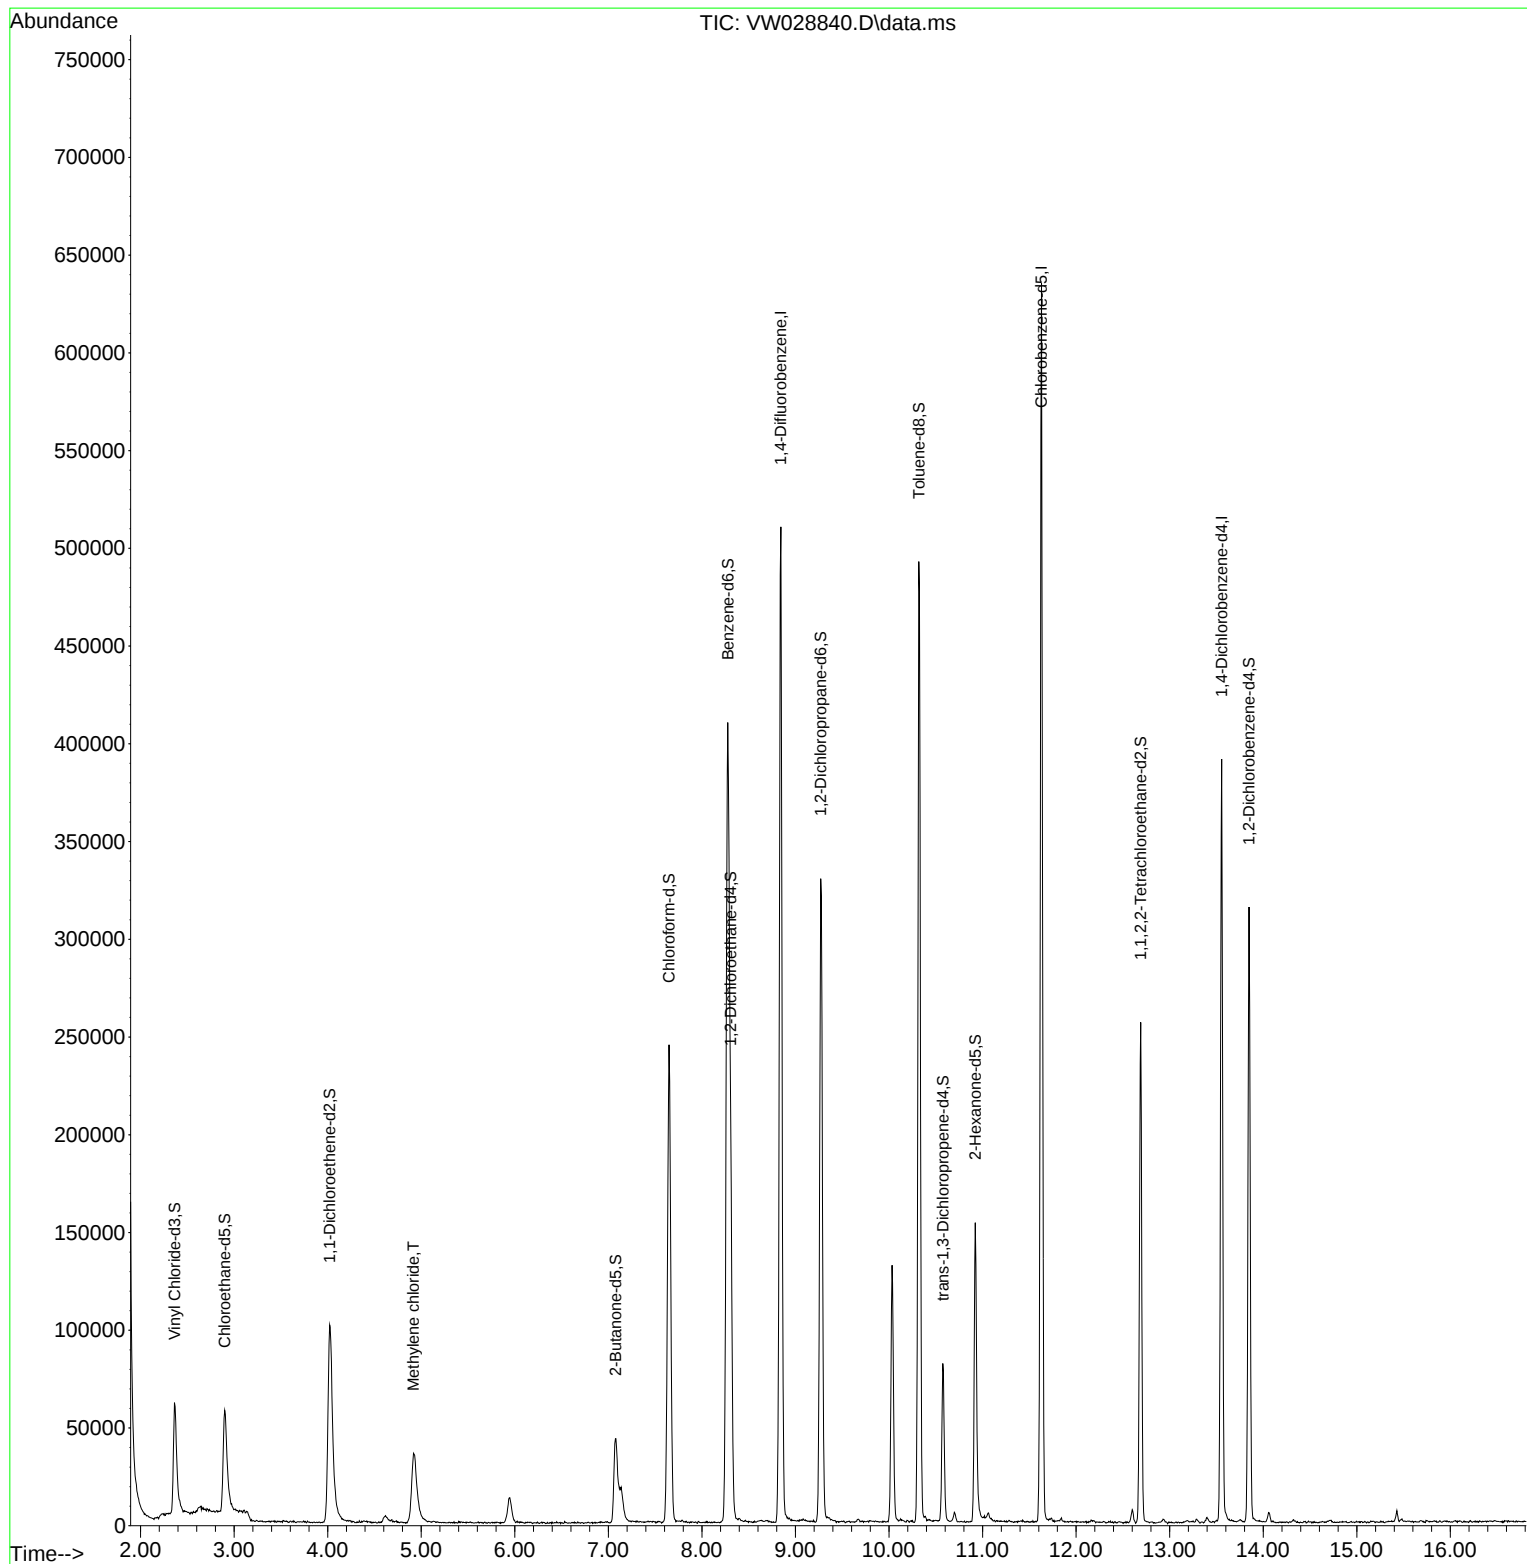

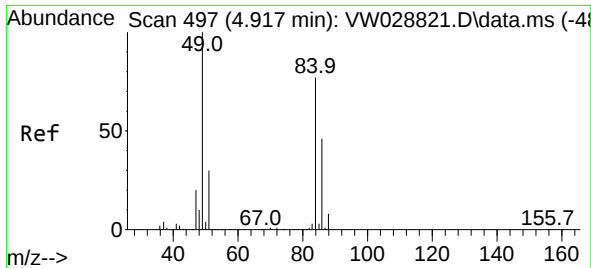

#16
Methylene chloride
Concen: 5.451 ug/L
RT: 4.917 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW028840.D
Acq: 28 May 2024 18:42

Instrument :
MSVOA_W
ClientSampleId :
BH5S8

Tgt Ion	Ratio	Lower	Upper
84	100		
86	59.5	44.4	82.4
49	128.1	100.2	186.2

