

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052824\
 Data File : VW028850.D
 Acq On : 28 May 2024 23:30
 Operator : SY/MD
 Sample : P2591-13
 Misc : 5.95g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BHBQ4

Quant Time: May 29 05:49:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 29 02:08:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	415373	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	362253	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	139394	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	97820	12.402	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	49.600%		
7) Chloroethane-d5	2.899	69	95169	15.758	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.040%		
11) 1,1-Dichloroethene-d2	4.027	65	46242	14.032	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.120%		
21) 2-Butanone-d5	7.075	46	82456	40.069	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	80.140%		
24) Chloroform-d	7.648	84	267556	20.614	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.440%		
26) 1,2-Dichloroethane-d4	8.307	65	155608	20.942	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.760%		
32) Benzene-d6	8.276	84	472909	19.567	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	78.280%		
36) 1,2-Dichloropropane-d6	9.276	67	166803	22.935	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.760%		
41) Toluene-d8	10.319	98	388877	18.169	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	72.680%		
43) trans-1,3-Dichloroprop...	10.575	79	53378	18.244	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	72.960%		
47) 2-Hexanone-d5	10.922	63	55001	43.848	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.700%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	143988	23.610	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.440%		
66) 1,2-Dichlorobenzene-d4	13.848	152	118929	22.385	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.520%		
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	42120	6.557	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052824\
Data File : VW028850.D
Acq On : 28 May 2024 23:30
Operator : SY/MD
Sample : P2591-13
Misc : 5.95g/10mL/MSVOA_W/SOIL/A
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BHBQ4

Quant Time: May 29 05:49:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 29 02:08:39 2024
Response via : Initial Calibration

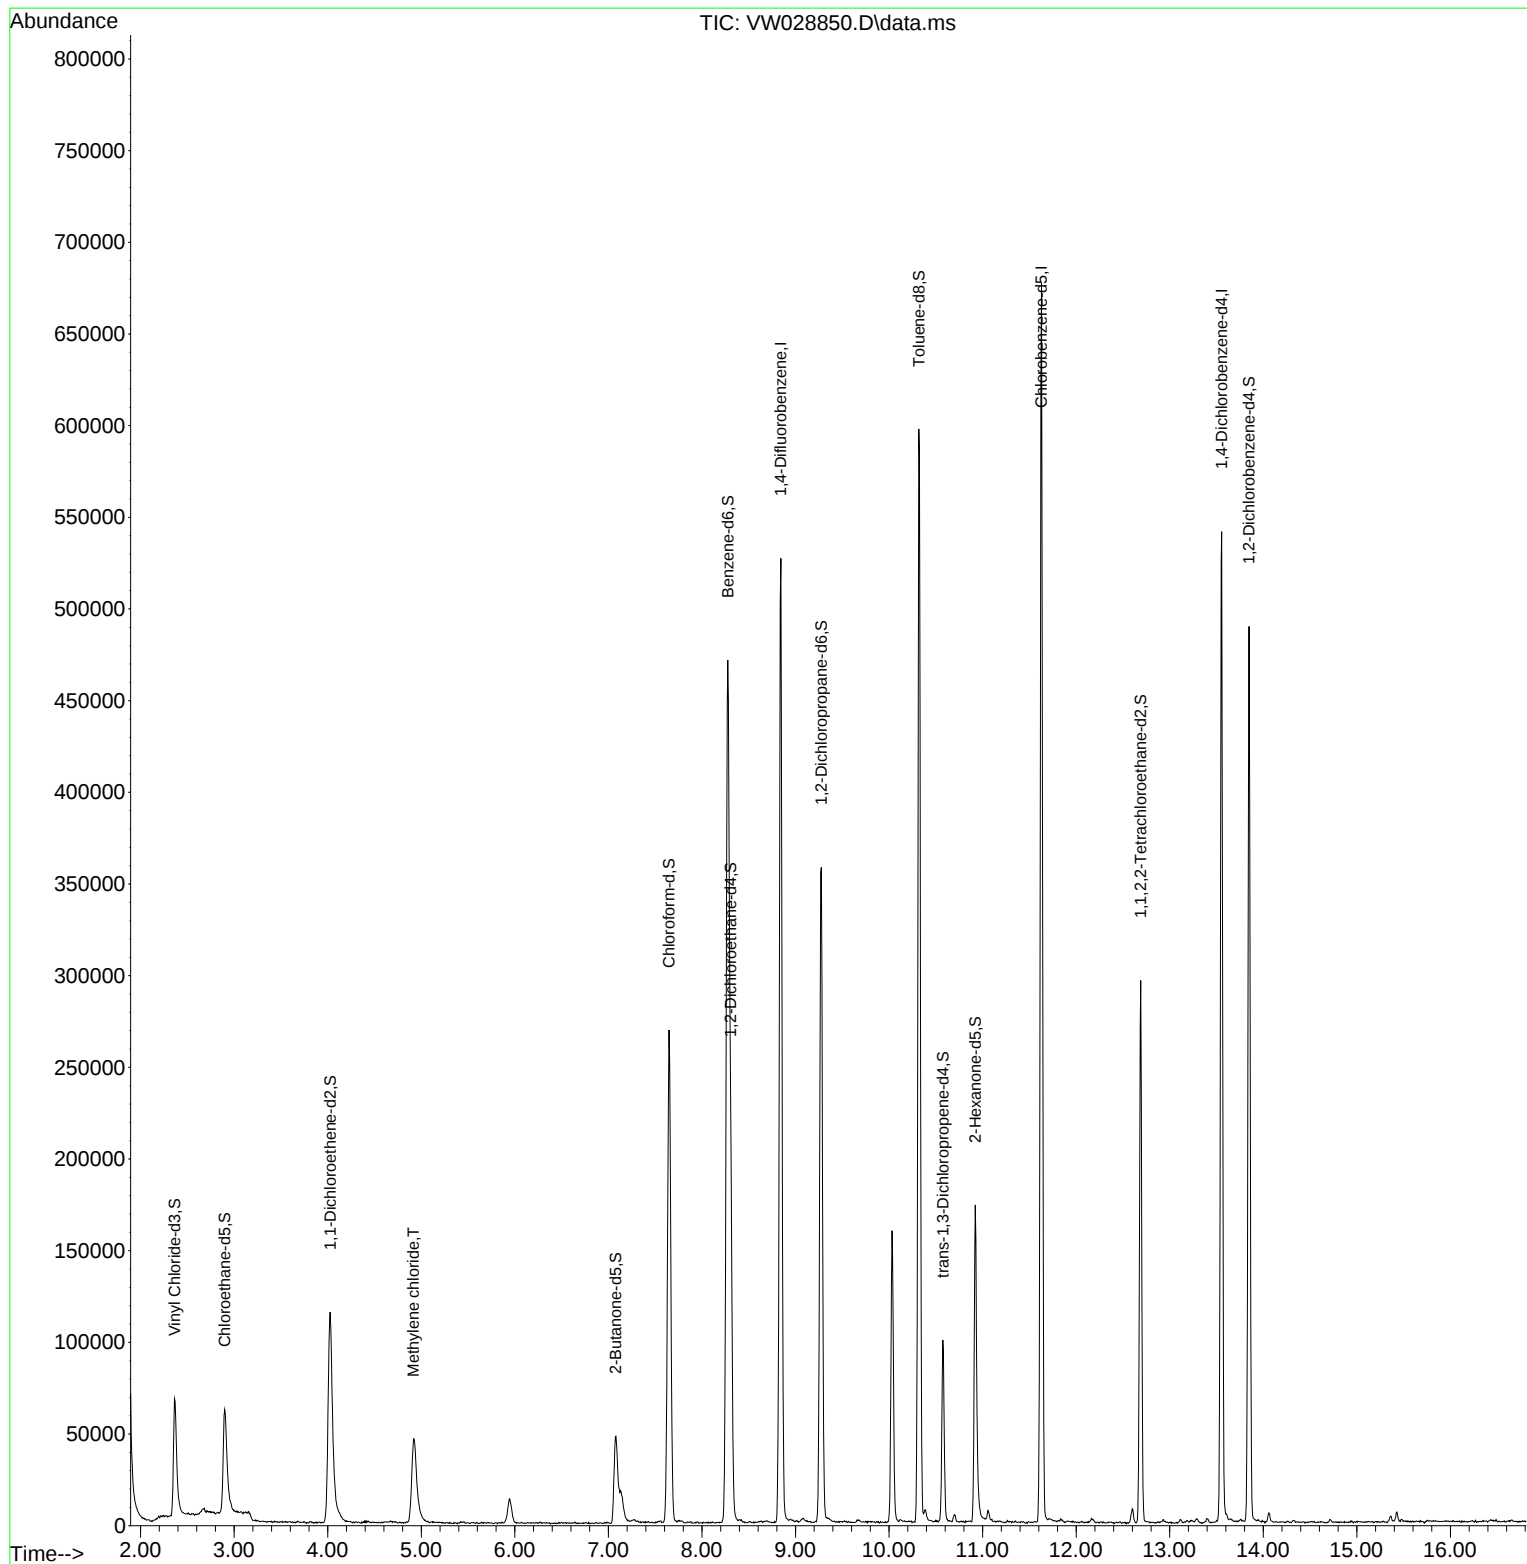

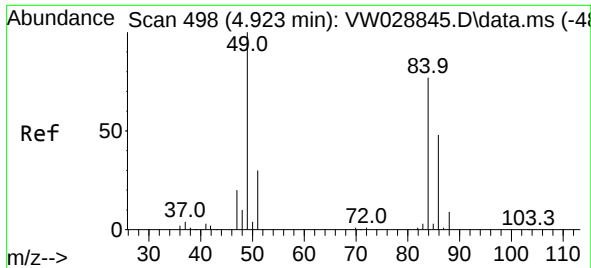

#16
Methylene chloride
Concen: 6.557 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW028850.D
Acq: 28 May 2024 23:30

Instrument :
MSVOA_W
ClientSampleId :
BHBQ4

Tgt Ion: 84 Resp: 42120
Ion Ratio Lower Upper
84 100
86 61.9 44.4 82.4
49 130.7 100.2 186.2

