

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052924\
 Data File : VW028873.D
 Acq On : 29 May 2024 10:51
 Operator : SY/MD
 Sample : P2571-21
 Misc : 5.07g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 30 01:30:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 29 23:53:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	291122	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	273090	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	123854	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	118657	21.464	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.840%
7) Chloroethane-d5	2.899	69	91047	21.509	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.040%
11) 1,1-Dichloroethene-d2	4.021	65	51403	22.255	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.040%
21) 2-Butanone-d5	7.075	46	60023	41.617	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.240%
24) Chloroform-d	7.648	84	225982	24.842	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.360%
26) 1,2-Dichloroethane-d4	8.306	65	128292	24.634	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.520%
32) Benzene-d6	8.276	84	450733	24.738	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.960%
36) 1,2-Dichloropropane-d6	9.276	67	139791	25.497	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.000%
41) Toluene-d8	10.318	98	398239	24.681	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.720%
43) trans-1,3-Dichloroprop...	10.580	79	53681	24.338	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.360%
47) 2-Hexanone-d5	10.922	63	38899	41.136	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.280%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	104141	22.652	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	128526	27.227	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.920%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	4472	0.676	ug/L	# 56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052924\
Data File : VW028873.D
Acq On : 29 May 2024 10:51
Operator : SY/MD
Sample : P2571-21
Misc : 5.07g/10mL/MSVOA_W/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 30 01:30:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 29 23:53:47 2024
Response via : Initial Calibration

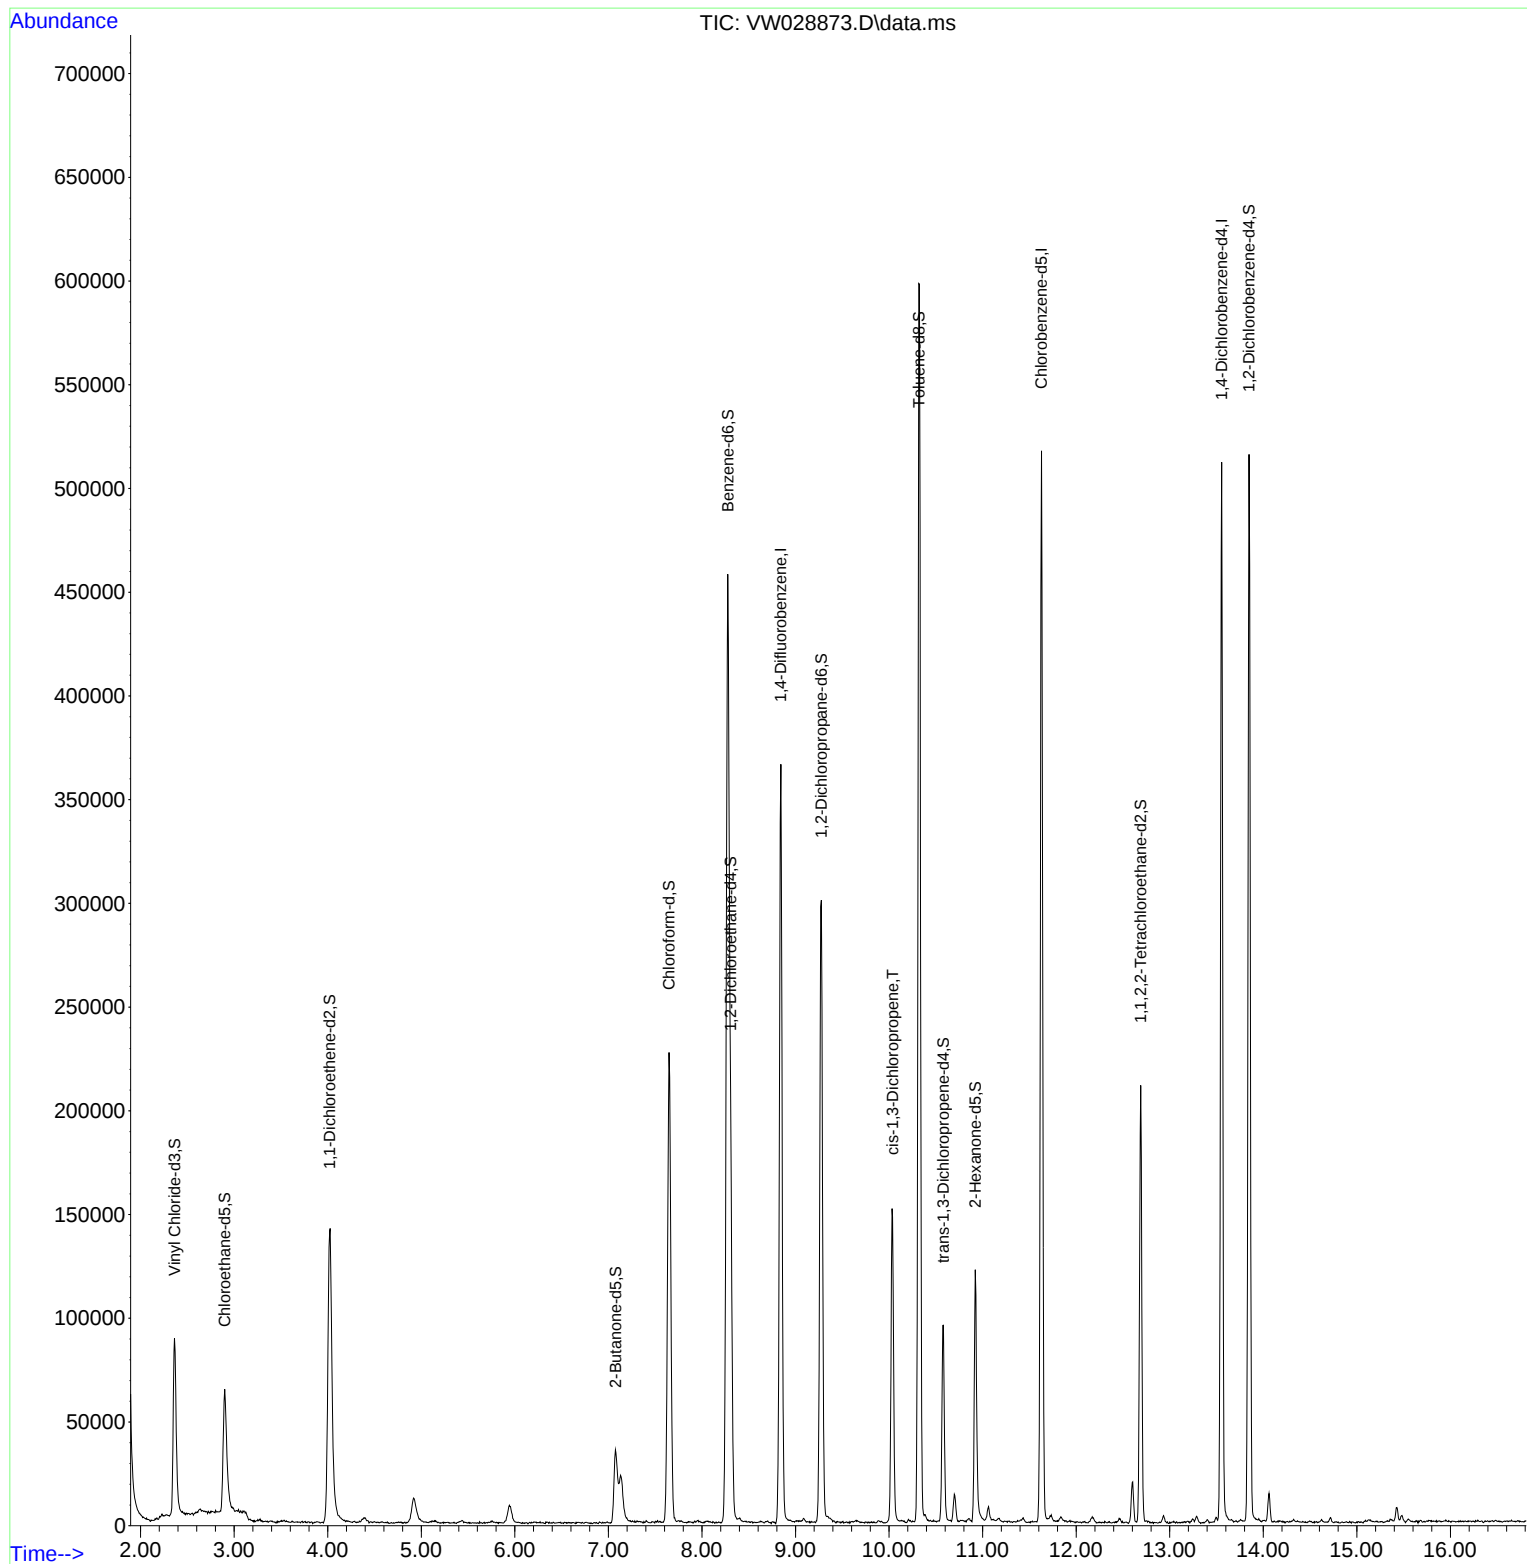

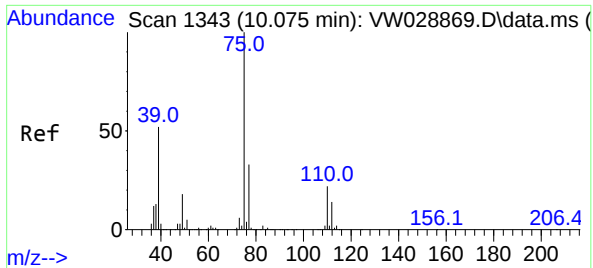

#39
 cis-1,3-Dichloropropene
 Concen: 0.676 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW028873.D
 Acq: 29 May 2024 10:51

Instrument :
 MSVOA_W
 ClientSampleId :

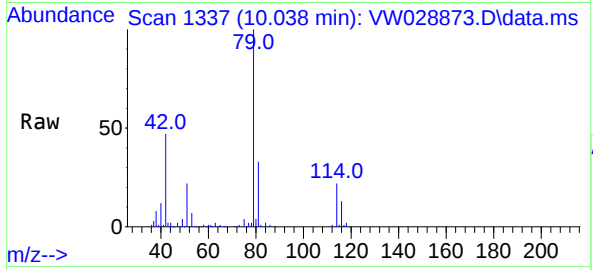

Tgt Ion: 75 Resp: 4472
 Ion Ratio Lower Upper
 75 100
 77 55.5 21.8 40.6#

