


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052924\
Data File : VW028868.D
Acq On : 29 May 2024 08:06
Operator : SY/MD
Sample : BFB494
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB494

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Title : SFAM01.0
Last Update : Wed May 29 23:53:47 2024

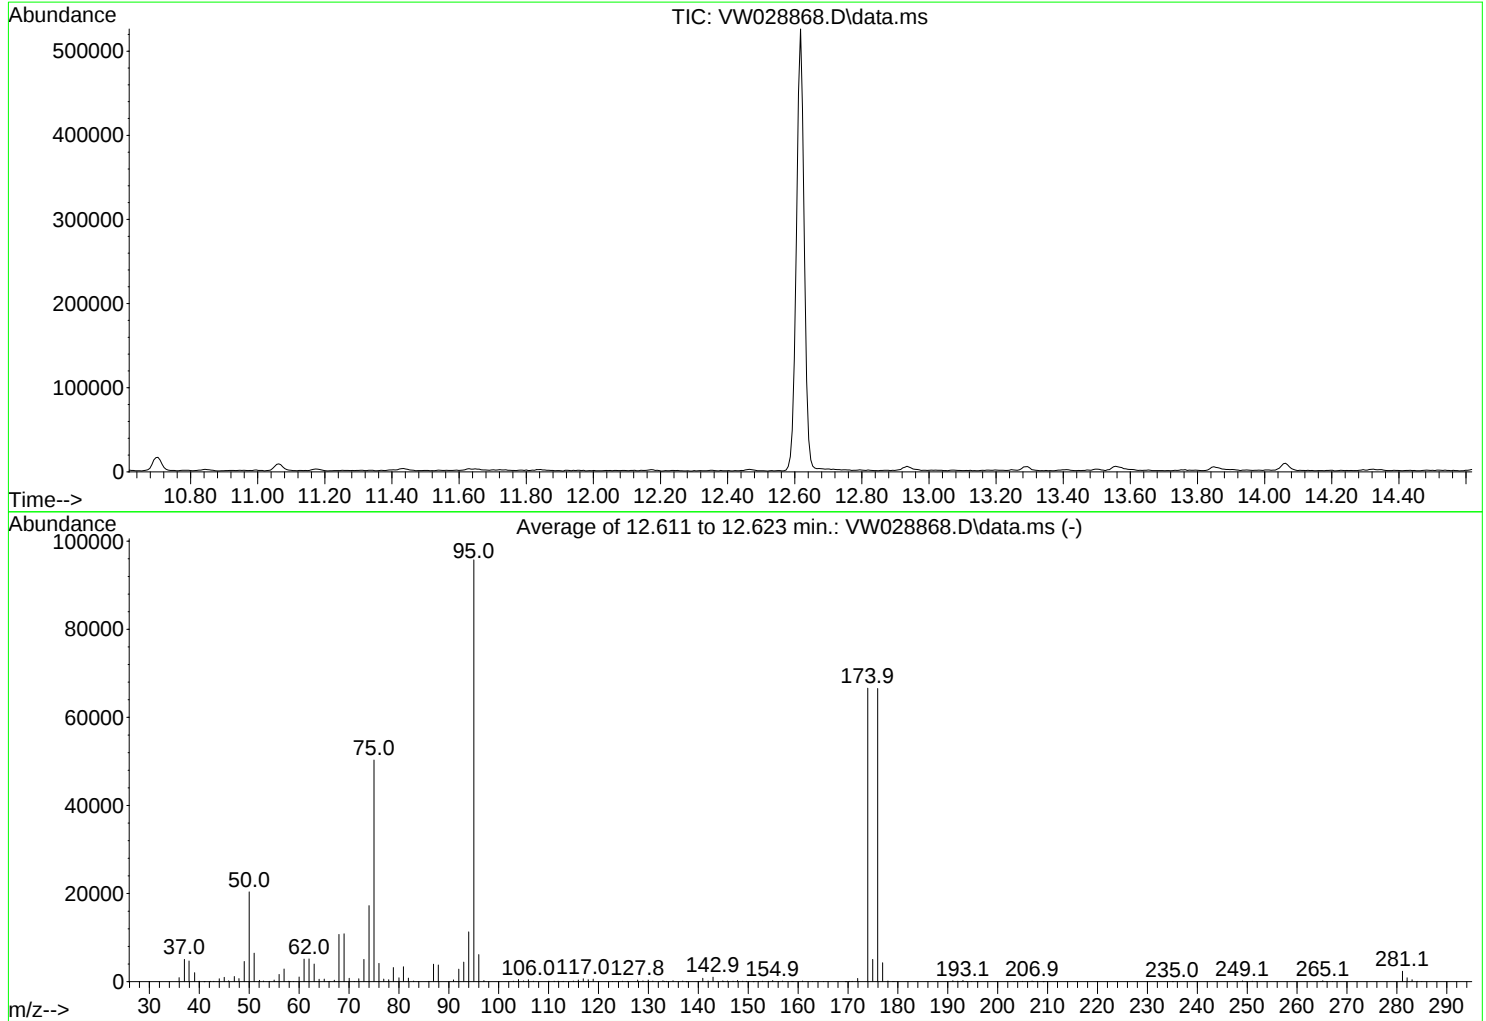

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	20394	PASS
75	95	30	80	52.5	50315	PASS
95	95	100	100	100.0	95768	PASS
96	95	5	9	6.4	6132	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.6	66616	PASS
175	174	5	9	7.6	5053	PASS
176	174	95	101	99.9	66552	PASS
177	176	5	9	6.5	4302	PASS

m/z	Abundance
35.10	66.0
35.50	83.0
35.90	73.0
37.90	94.0
38.60	70.0
40.00	254.0
41.00	75.0
41.60	75.0
42.90	55.0
44.00	259.0
46.90	89.0
50.20	51.0
95.30	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB494

m/z	Abundance
36.00	948.0
37.00	5061.0
38.00	4882.0
39.10	2201.0
39.90	404.0
40.90	76.0
43.00	127.0
44.00	836.0
45.00	1123.0
45.90	165.0
47.10	1280.0
48.00	721.0
49.00	4436.0
50.00	19872.0
51.00	6869.0
52.00	244.0
52.80	150.0
54.00	77.0
55.00	357.0
56.00	1664.0
57.00	2787.0
57.90	141.0
58.80	87.0
60.00	1072.0
61.00	5438.0
62.00	5231.0
63.00	3888.0
64.00	555.0
65.10	602.0
65.80	126.0
67.00	357.0
68.00	10510.0
69.00	10759.0
70.10	744.0
72.00	575.0
73.00	5167.0
74.00	16888.0
75.00	48720.0
76.00	4063.0
76.90	516.0
77.90	417.0
78.90	3325.0
80.00	932.0
80.90	3258.0
81.90	831.0
83.00	154.0
83.90	61.0
86.00	169.0
86.90	4100.0
87.90	3574.0
91.00	317.0
92.00	2604.0
93.00	4484.0
94.00	10823.0
95.00	90800.0
96.00	6288.0
97.10	250.0
103.00	166.0
104.00	524.0
105.10	217.0
106.00	358.0
106.90	110.0
110.10	113.0
111.10	74.0
112.00	143.0
112.70	132.0
114.90	156.0
116.00	276.0
117.00	673.0
118.00	472.0
119.00	542.0
124.90	148.0
125.90	113.0
127.90	396.0
128.90	205.0
130.00	346.0
130.90	171.0
132.90	347.0
133.60	233.0
135.00	225.0
137.00	160.0
137.60	51.0
140.90	625.0
142.00	126.0
143.00	1015.0
143.90	73.0
144.90	295.0
145.90	127.0
146.90	115.0
147.90	282.0
149.00	115.0
149.70	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB494

152.90	64.0
154.10	77.0
155.00	228.0
156.00	87.0
156.80	138.0
158.80	135.0
160.90	170.0
162.90	86.0
165.10	65.0
170.30	69.0
172.00	625.0
173.90	59744.0
175.00	4575.0
176.00	59888.0
176.90	3923.0
178.00	141.0
179.00	138.0
191.00	336.0
192.10	97.0
193.10	612.0
193.70	65.0
194.80	58.0
195.90	51.0
203.30	60.0
205.00	147.0
206.90	323.0
208.00	74.0
235.00	52.0
249.10	235.0
249.80	85.0
251.00	170.0
251.90	70.0
265.20	324.0
265.90	70.0
267.10	113.0
281.10	3142.0
282.10	1318.0
283.10	665.0
284.10	180.0
285.00	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB494

m/z	Abundance
36.00	1066.0
37.00	5765.0
38.00	5265.0
39.00	2176.0
39.90	356.0
40.90	116.0
42.20	64.0
43.00	148.0
44.00	1023.0
45.00	1026.0
46.00	176.0
47.00	1490.0
48.00	693.0
49.00	5072.0
50.00	23472.0
51.00	7237.0
52.10	373.0
52.90	183.0
54.00	86.0
55.00	419.0
56.00	1814.0
57.00	3149.0
57.90	98.0
58.20	95.0
58.90	63.0
60.00	1186.0
61.00	5839.0
62.00	6108.0
63.00	4673.0
64.00	649.0
65.00	692.0
66.20	110.0
67.10	320.0
68.00	11768.0
69.00	12257.0
70.10	826.0
71.00	67.0
71.90	721.0
73.00	5844.0
74.00	19232.0
75.00	56728.0
76.00	4729.0
76.90	621.0
77.90	497.0
78.90	3614.0
80.00	974.0
80.90	3852.0
81.90	964.0
82.90	165.0
87.00	4359.0
87.90	4371.0
91.00	492.0
92.00	3279.0
93.00	4858.0
94.00	12706.0
95.00	107296.0
96.00	6946.0
97.00	268.0
102.90	134.0
103.90	411.0
104.90	251.0
106.00	440.0
107.00	116.0
110.00	156.0
111.00	115.0
111.80	133.0
113.00	131.0
114.90	178.0
116.00	434.0
116.90	644.0
118.00	440.0
118.90	773.0
122.80	69.0
124.80	73.0
125.70	82.0
127.90	427.0
128.90	162.0
129.90	379.0
130.90	122.0
132.90	284.0
134.00	96.0
135.00	234.0
136.80	171.0
140.80	936.0
142.00	178.0
142.80	1038.0
143.70	91.0
145.10	273.0
145.80	165.0
147.00	156.0
147.90	307.0
148.80	148.0

Instrument :
MSVOA_W
ClientSampleId :
BFB494

149.70	101.0
150.10	117.0
152.90	153.0
153.90	60.0
154.80	281.0
156.10	62.0
156.90	204.0
158.60	80.0
159.10	94.0
160.80	151.0
165.10	55.0
170.20	111.0
170.90	123.0
172.00	889.0
174.00	76168.0
174.90	5631.0
175.90	73000.0
177.00	4787.0
178.00	200.0
179.20	78.0
191.00	276.0
192.00	119.0
193.00	215.0
194.80	65.0
203.20	59.0
204.90	52.0
206.90	129.0
207.90	95.0
209.10	56.0
249.00	227.0
251.10	90.0
251.90	53.0
265.10	304.0
266.00	82.0
267.10	52.0
281.10	2581.0
282.00	882.0
283.00	449.0
285.00	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB494

m/z	Abundance
36.00	887.0
37.00	4365.0
38.00	4228.0
39.00	1723.0
40.00	361.0
41.00	74.0
41.50	65.0
42.30	105.0
42.80	119.0
44.10	910.0
45.00	809.0
45.80	189.0
47.00	1004.0
47.80	645.0
49.00	4194.0
50.00	17992.0
51.00	5337.0
52.00	228.0
52.90	96.0
54.10	67.0
55.00	349.0
56.00	1469.0
57.00	2668.0
58.00	110.0
60.00	873.0
61.00	4129.0
62.00	4142.0
63.00	3393.0
64.00	457.0
65.00	476.0
66.10	94.0
67.10	355.0
68.00	9848.0
69.00	9603.0
70.00	709.0
71.10	77.0
72.00	678.0
73.00	4194.0
74.00	15655.0
75.00	45496.0
76.00	3595.0
77.00	635.0
78.00	447.0
78.90	2690.0
80.00	735.0
80.90	3068.0
81.90	648.0
82.90	99.0
87.00	3422.0
87.90	3442.0
90.90	398.0
92.00	2608.0
93.00	3926.0
94.00	10379.0
95.00	89208.0
96.00	5163.0
97.00	219.0
102.90	80.0
103.90	477.0
104.90	131.0
105.90	506.0
107.00	93.0
110.10	72.0
111.20	148.0
112.00	82.0
113.00	108.0
115.00	155.0
115.90	368.0
117.00	630.0
117.90	352.0
118.90	481.0
124.90	110.0
127.80	323.0
128.90	173.0
129.90	368.0
130.90	103.0
133.20	172.0
133.90	59.0
134.90	220.0
136.90	136.0
140.00	83.0
141.00	745.0
141.90	133.0
143.00	1040.0
143.80	66.0
144.90	218.0
145.90	165.0
146.90	96.0
147.80	232.0
149.00	65.0
149.80	57.0
151.00	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB494

152.10	80.0
152.90	66.0
154.10	57.0
154.90	249.0
157.00	159.0
158.90	129.0
161.00	126.0
169.50	55.0
170.70	98.0
171.90	719.0
174.00	63936.0
175.00	4952.0
175.90	66768.0
177.00	4196.0
178.00	161.0
190.90	74.0
191.90	61.0
192.80	133.0
207.20	134.0
249.00	112.0
250.90	75.0
264.80	154.0
281.10	1323.0
282.10	457.0
282.90	173.0
284.00	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB494