

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW053123\
 Data File : VW026102.D
 Acq On : 31 May 2023 16:48
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK465

Quant Time: Jun 01 01:28:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 01 01:27:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	682881	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	618413	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	274549	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	257760	26.831	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.320%
7) Chloroethane-d5	2.893	69	173666	24.149	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.600%
11) 1,1-Dichloroethene-d2	4.021	65	126956	26.801	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	107.200%
21) 2-Butanone-d5	7.075	46	137162	49.042	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.080%
24) Chloroform-d	7.648	84	480429	24.025	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.080%
26) 1,2-Dichloroethane-d4	8.228	65	88	0.008	ug/L	-0.07
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.270	84	1003961	24.127	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.520%
36) 1,2-Dichloropropane-d6	9.270	67	301305	22.855	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.440%
41) Toluene-d8	10.319	98	789664	21.398	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.600%
43) trans-1,3-Dichloroprop...	10.575	79	99950	19.133	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.520%
47) 2-Hexanone-d5	10.922	63	82545	39.710	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.420%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	226549	23.615	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.480%
66) 1,2-Dichlorobenzene-d4	13.849	152	258100	24.561	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.240%
Target Compounds					Qvalue	
48) 2-Hexanone	10.922	43	11360	2.382	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW053123\
Data File : VW026102.D
Acq On : 31 May 2023 16:48
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK465

Quant Time: Jun 01 01:28:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 01 01:27:52 2023
Response via : Initial Calibration

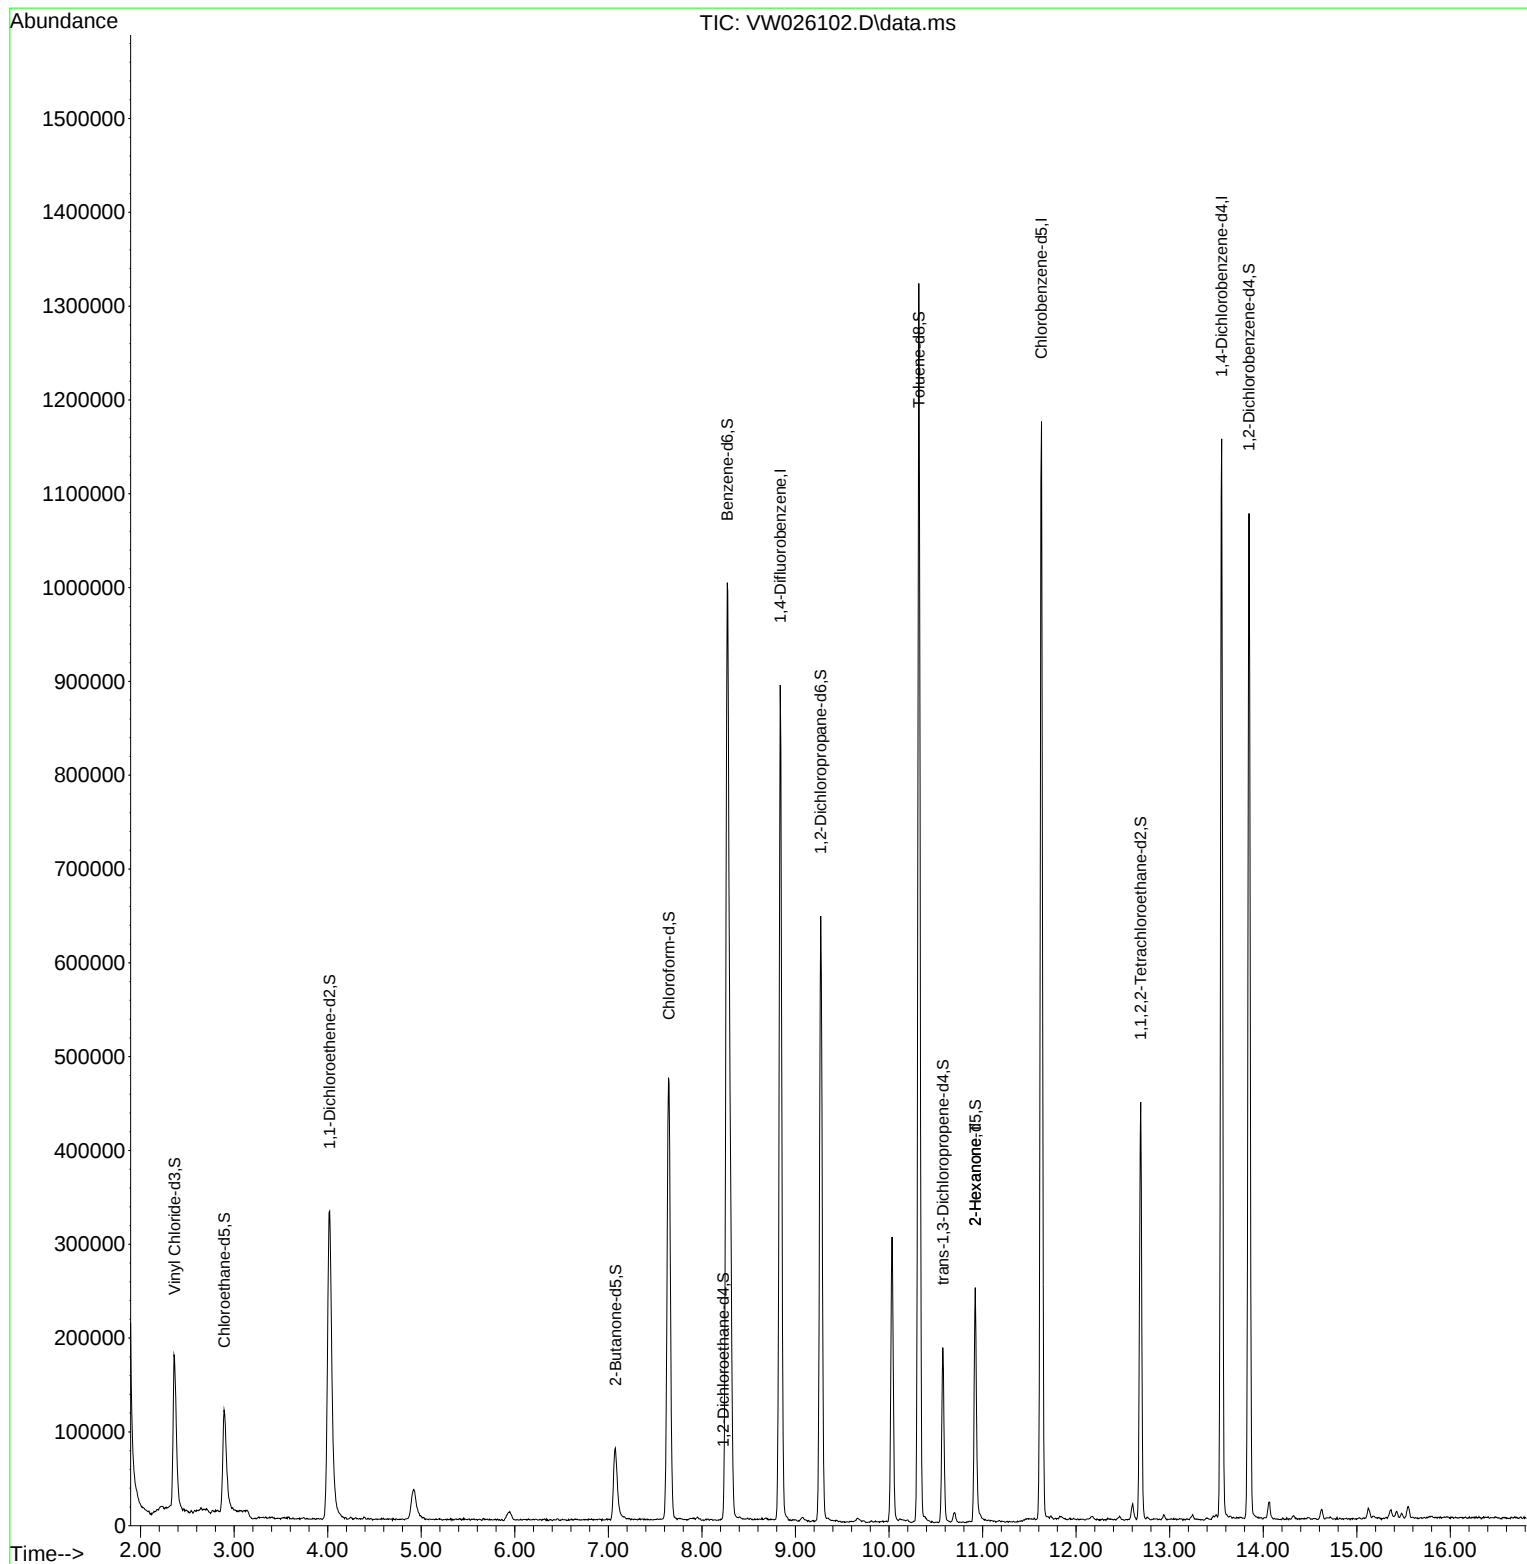

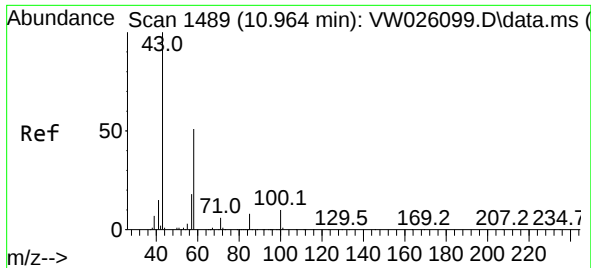

#48

2-Hexanone

Concen: 2.382 ug/L

RT: 10.922 min Scan# 14

Delta R.T. -0.042 min

Lab File: VW026102.D


Acq: 31 May 2023 16:48

Instrument :

MSVOA_W

ClientSampleId :

VIBLK465

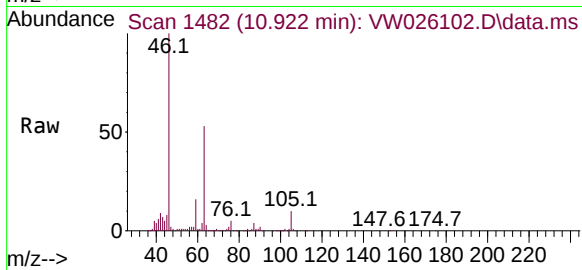

Tgt Ion: 43 Resp: 11360

Ion Ratio Lower Upper

43 100

58 24.1 42.2 63.2#

57 29.9 14.2 21.2#

100 3.4 8.3 12.5#

