

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060222\
 Data File : VW023381.D
 Acq On : 02 Jun 2022 17:52
 Operator : SY/VA
 Sample : N3171-10
 Misc : 6.34g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBTZ5

Quant Time: Jun 02 21:59:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 02 21:56:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	402608	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	370431	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	156194	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	160918	27.027	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.120%
7) Chloroethane-d5	2.879	69	96902	23.410	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.640%
11) 1,1-Dichloroethene-d2	4.013	63	149373	16.322	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.280%
21) 2-Butanone-d5	7.074	46	63597	51.896	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.800%
24) Chloroform-d	7.647	84	224148	21.142	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.560%
26) 1,2-Dichloroethane-d4	8.305	65	131865	23.747	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.000%
32) Benzene-d6	8.274	84	446581	22.437	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.760%
36) 1,2-Dichloropropane-d6	9.274	67	129721	22.781	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.120%
41) Toluene-d8	10.323	98	428397	22.574	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.280%
43) trans-1,3-Dichloroprop...	10.579	79	55179	21.707	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.840%
47) 2-Hexanone-d5	10.920	63	48551	53.074	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.140%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	118793	23.653	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	128736	23.317	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.280%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4844	0.617	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060222\
Data File : VW023381.D
Acq On : 02 Jun 2022 17:52
Operator : SY/VA
Sample : N3171-10
Misc : 6.34g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBTZ5

Quant Time: Jun 02 21:59:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 02 21:56:41 2022
Response via : Initial Calibration

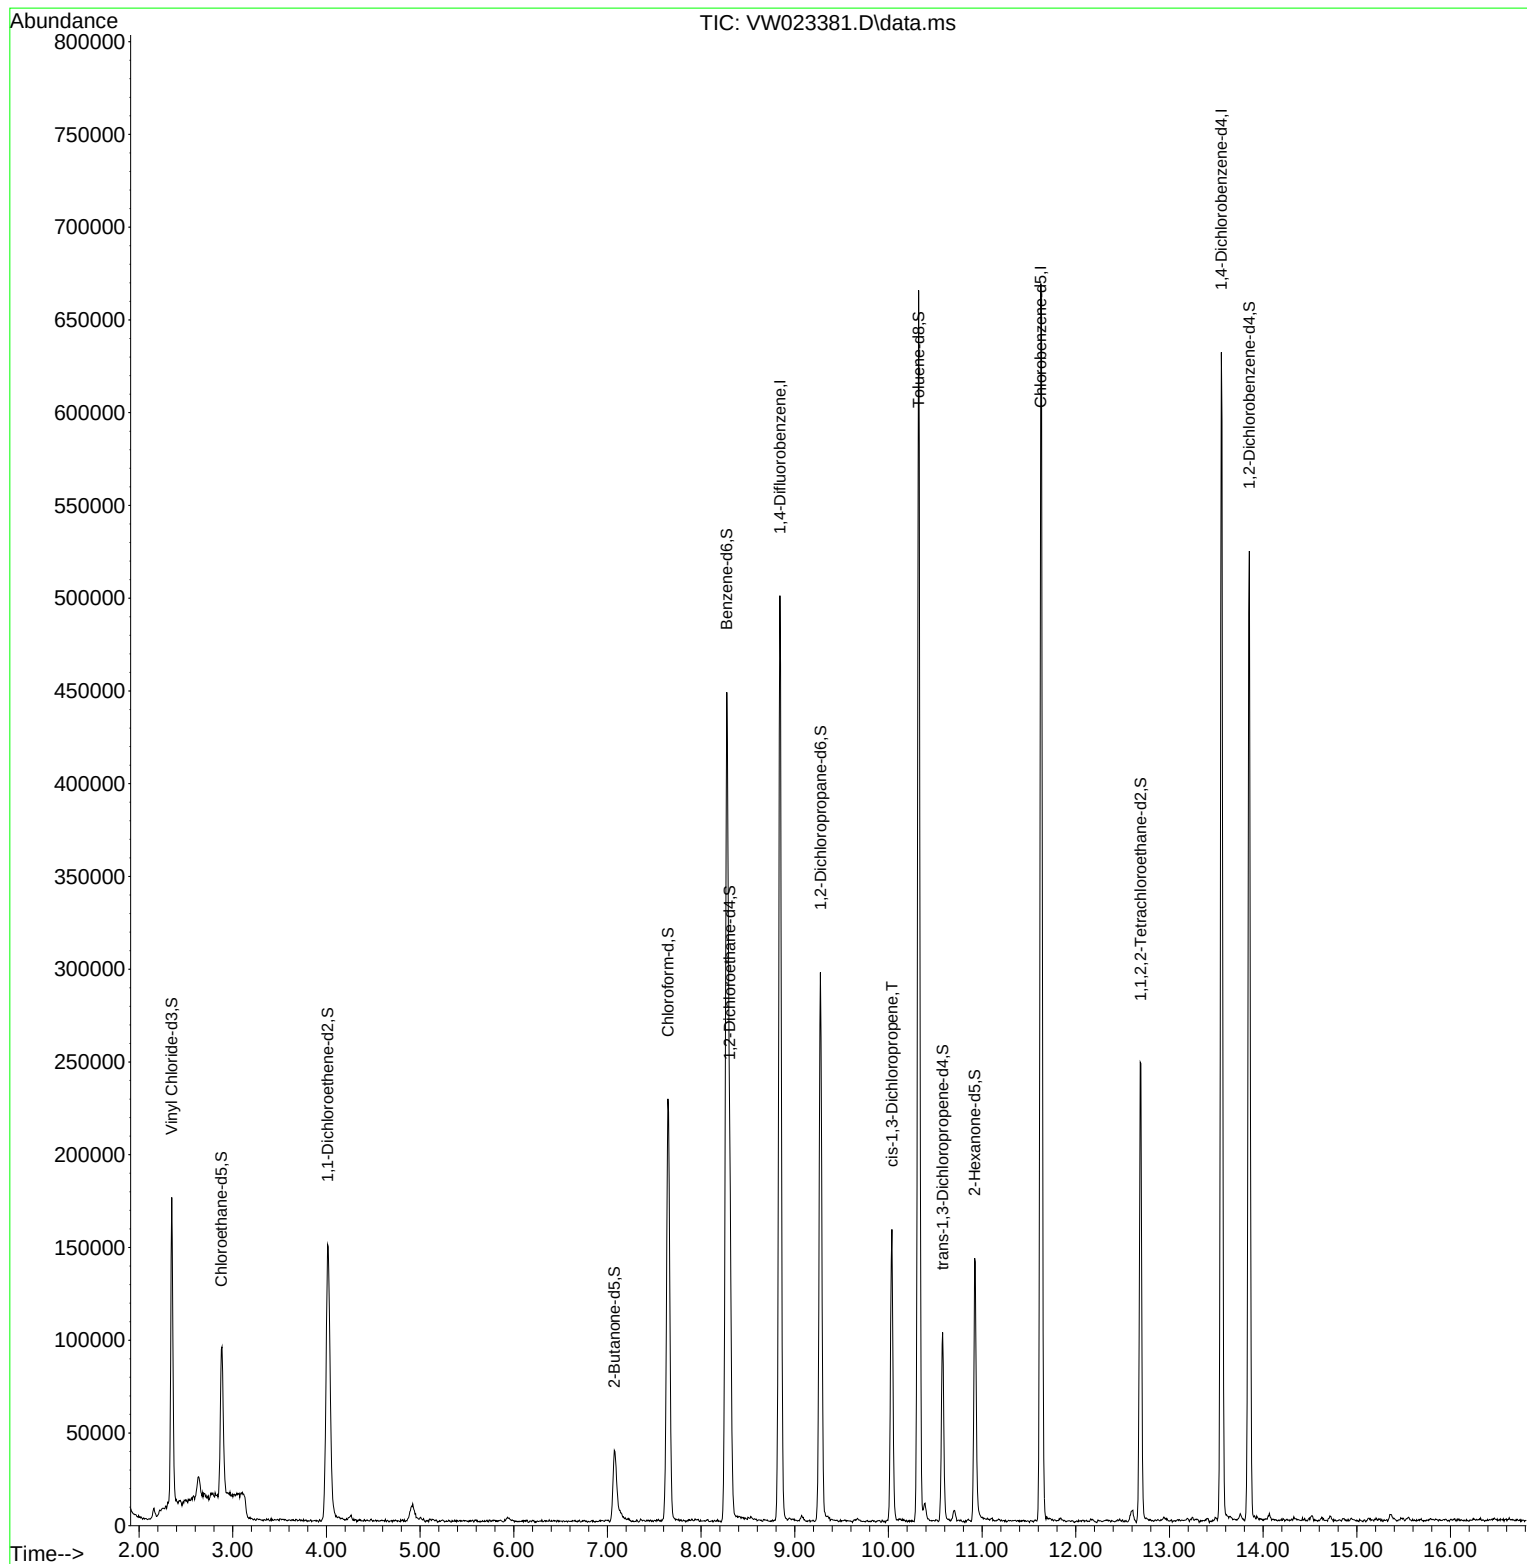

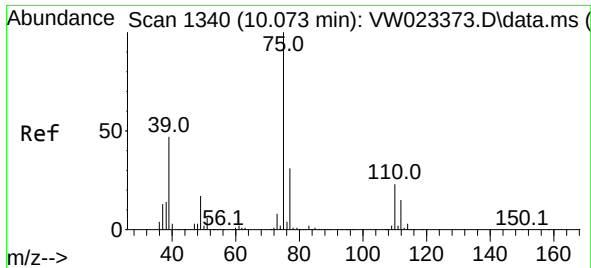

#39
 cis-1,3-Dichloropropene
 Concen: 0.617 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023381.D
 Acq: 02 Jun 2022 17:52

Instrument :
 MSVOA_W
 ClientSampleId :
 DBTZ5

Tgt Ion: 75 Resp: 4844
 Ion Ratio Lower Upper
 75 100
 77 48.8 22.1 41.1#

