

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060222\
 Data File : VW023382.D
 Acq On : 02 Jun 2022 18:16
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK490

Quant Time: Jun 02 21:59:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 02 21:56:41 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	362815	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.634	117	345576	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	159604	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	147046	27.406	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.640%	
7) Chloroethane-d5		2.885	69	84510	22.655	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.640%	
11) 1,1-Dichloroethene-d2		4.013	63	140987	17.096	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.400%	
21) 2-Butanone-d5		7.074	46	59953	54.288	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.580%	
24) Chloroform-d		7.653	84	237796	24.890	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.560%	
26) 1,2-Dichloroethane-d4		8.421	65	113	0.023	ug/L	0.12
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#	
32) Benzene-d6		8.275	84	448682	24.164	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.640%	
36) 1,2-Dichloropropane-d6		9.274	67	135526	25.512	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.040%	
41) Toluene-d8		10.323	98	445694	25.175	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.680%	
43) trans-1,3-Dichloroprop...		10.579	79	58365	24.612	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.440%	
47) 2-Hexanone-d5		10.920	63	48114	56.379	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.760%	
56) 1,1,2,2-Tetrachloroeth...		12.688	84	117977	25.180	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.720%	
66) 1,2-Dichlorobenzene-d4		13.853	152	150023	26.592	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.360%	
Target Compounds							Qvalue
34) Trichloroethene		8.842	95	11646	2.172	ug/L	# 4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060222\
Data File : VW023382.D
Acq On : 02 Jun 2022 18:16
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK490

Quant Time: Jun 02 21:59:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 02 21:56:41 2022
Response via : Initial Calibration

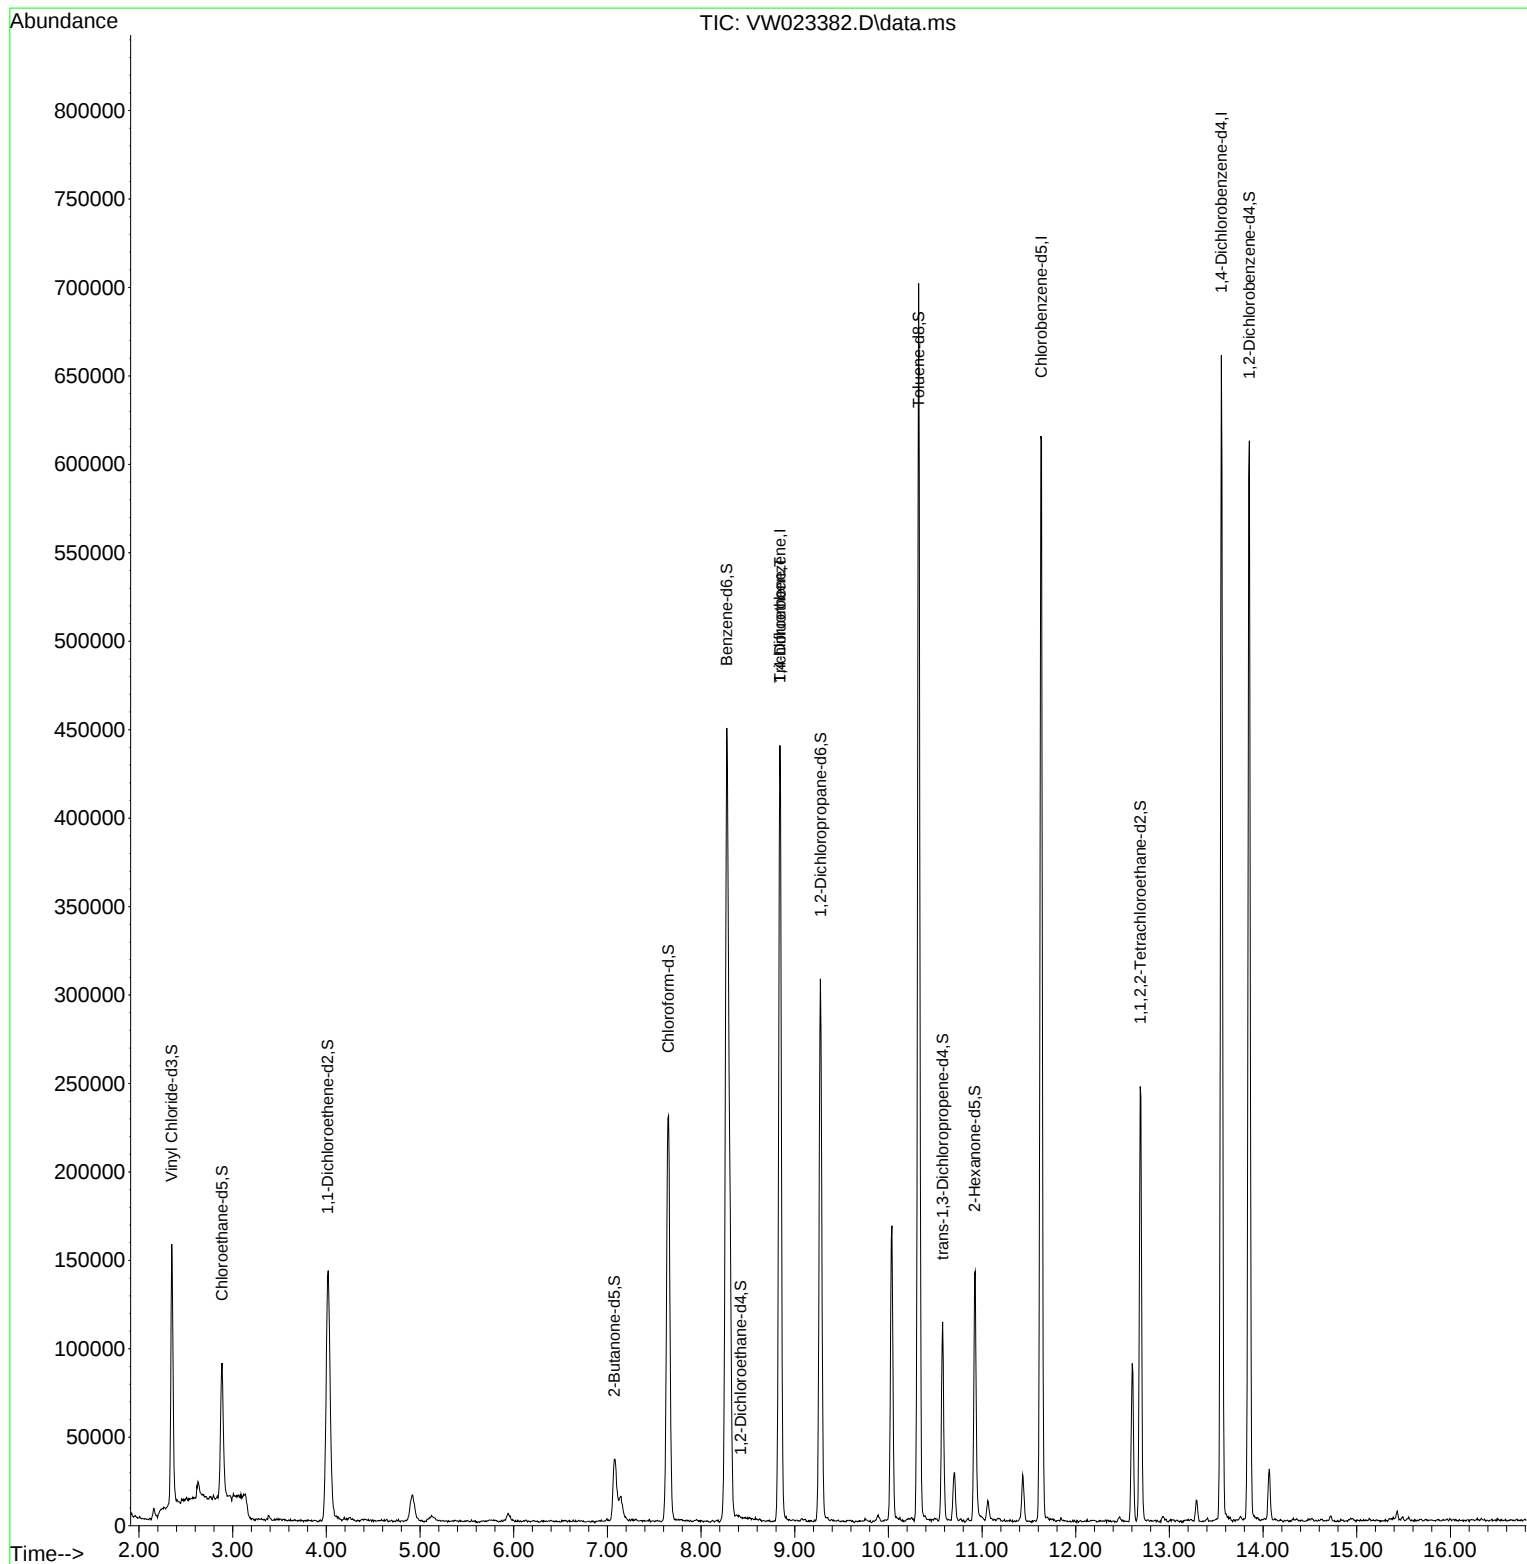

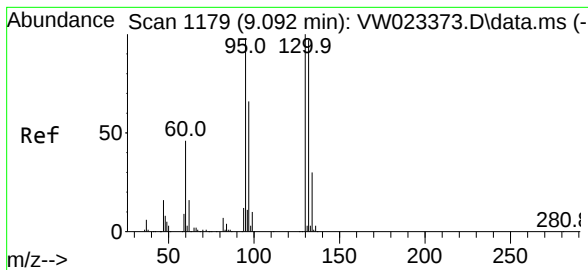

#34

Trichloroethene

Concen: 2.172 ug/L

RT: 8.842 min Scan# 11

Delta R.T. -0.250 min

Lab File: VW023382.D


Acq: 02 Jun 2022 18:16

Instrument :

MSVOA_W

ClientSampleId :

VIBLK490

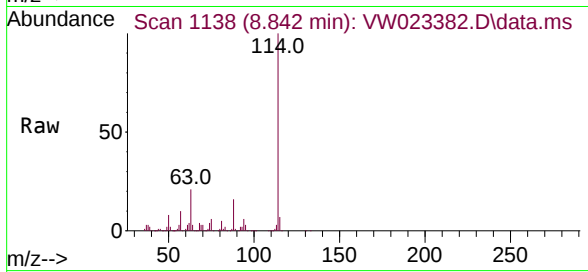

Tgt Ion: 95 Resp: 11646

Ion Ratio Lower Upper

95 100

97 0.0 43.8 81.3#

132 0.0 68.9 127.9#

130 1.0 75.3 139.8#

