


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060321\
Data File : VW019103.D
Acq On : 03 Jun 2021 09:56
Operator : SY/VA
Sample : BFB01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB101

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Title : SFAM01.0
Last Update : Sat Jun 05 00:35:45 2021

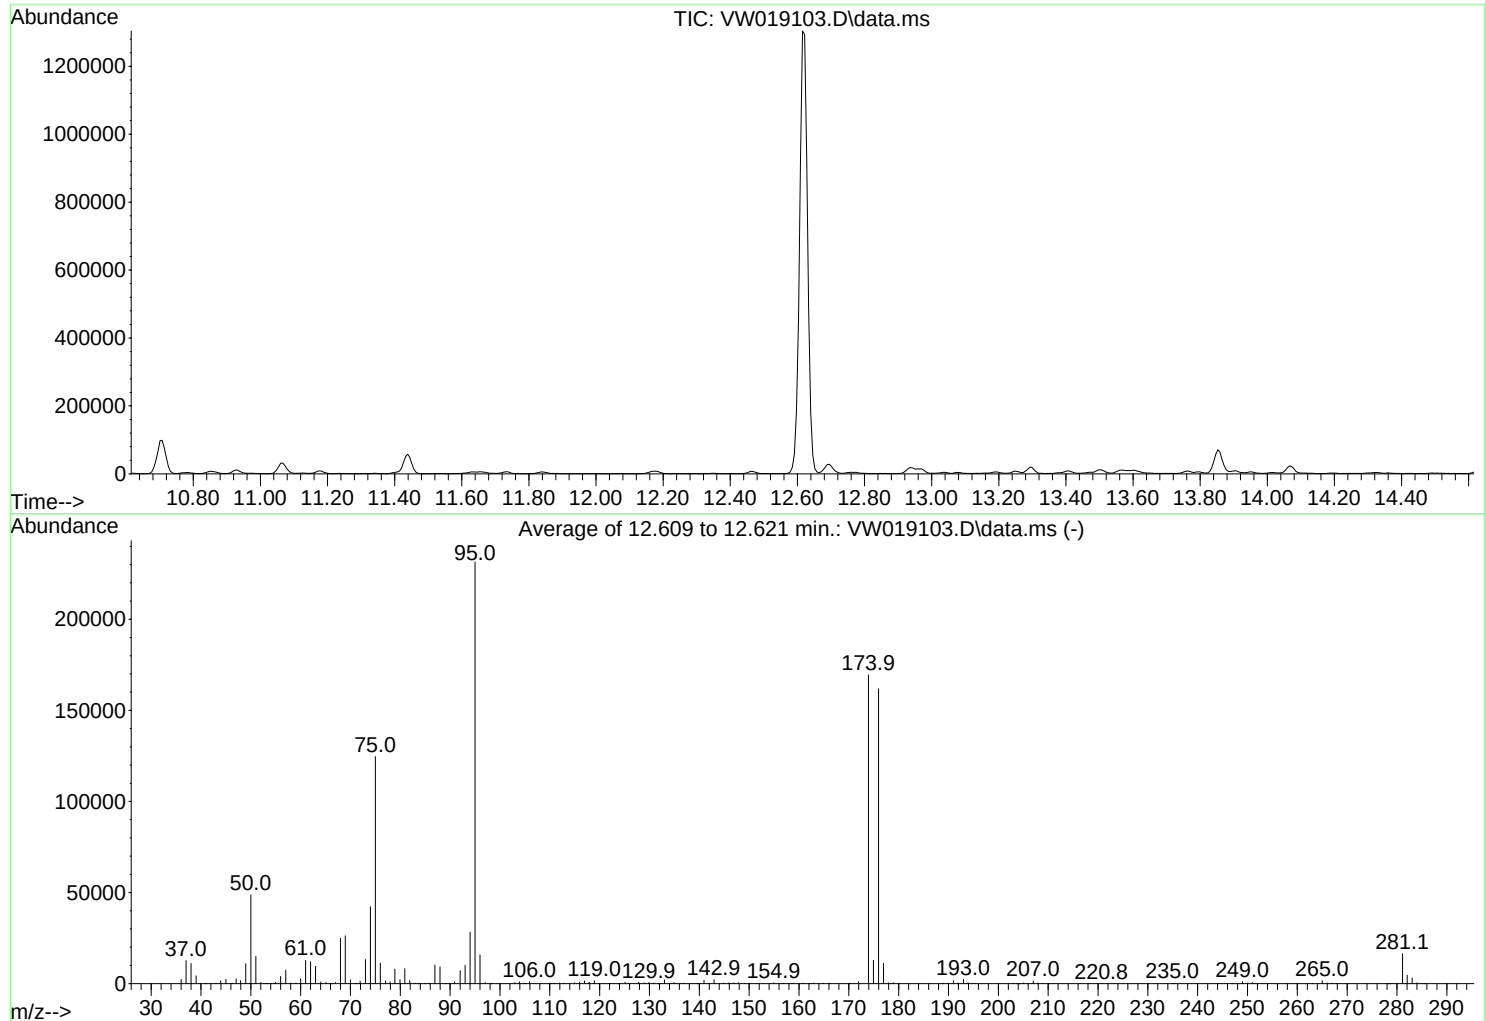

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	48776	PASS
75	95	30	80	53.8	124643	PASS
95	95	100	100	100.0	231531	PASS
96	95	5	9	6.8	15844	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.2	169469	PASS
175	174	5	9	7.6	12805	PASS
176	174	95	105	95.5	161829	PASS
177	176	5	10	6.9	11130	PASS

m/z	Abundance
39.90	306.0
41.00	84.0
42.00	77.0
43.10	71.0
43.90	334.0
57.10	103.0
68.90	97.0
169.00	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB101

142.90	2785.0
144.00	114.0
144.90	410.0
145.90	293.0
146.90	333.0
147.90	536.0
149.10	263.0
149.90	344.0
152.00	87.0
152.90	162.0
154.00	98.0
155.00	512.0
155.90	154.0
156.80	481.0
157.80	93.0
158.90	324.0
160.90	317.0
163.00	190.0
164.80	150.0
169.00	80.0
170.00	56.0
171.10	154.0
172.00	1037.0
173.90	205312.0
175.00	15001.0
175.90	190272.0
176.90	13738.0
178.00	443.0
178.70	159.0
179.10	213.0
189.00	160.0
191.00	1067.0
192.10	209.0
193.00	1269.0
194.00	273.0
195.20	146.0
203.10	190.0
205.10	233.0
206.00	94.0
207.00	804.0
207.80	253.0
209.00	130.0
234.90	69.0
235.20	80.0
249.10	1005.0
249.90	246.0
250.90	275.0
252.10	70.0
252.90	102.0
265.10	812.0
266.00	151.0
267.00	208.0
281.10	11371.0
282.10	3186.0
283.10	2093.0
284.00	482.0
285.00	193.0

Instrument :
MSVOA_W
ClientSampleId :
BFB101

135.90	69.0
136.90	404.0
138.60	83.0
139.60	61.0
141.00	1983.0
141.90	335.0
142.90	2174.0
144.90	417.0
145.90	349.0
146.90	521.0
147.80	582.0
149.10	258.0
150.00	333.0
151.90	112.0
152.90	163.0
154.00	130.0
154.90	506.0
156.00	117.0
156.90	428.0
158.00	125.0
158.80	305.0
160.80	326.0
161.90	53.0
162.80	320.0
163.90	132.0
164.90	280.0
168.90	182.0
170.20	61.0
171.00	169.0
172.00	1027.0
174.00	185792.0
175.00	13819.0
176.00	185216.0
176.90	11331.0
177.90	496.0
179.00	510.0
180.10	61.0
189.10	176.0
191.00	1722.0
191.90	336.0
193.00	2709.0
194.00	373.0
194.90	174.0
202.90	262.0
205.00	582.0
206.10	141.0
207.00	1515.0
207.90	503.0
208.80	144.0
220.70	80.0
234.90	201.0
249.00	1242.0
250.00	446.0
250.90	582.0
252.90	57.0
263.00	66.0
265.00	1809.0
266.00	575.0
266.90	376.0
267.80	152.0
278.60	81.0
279.20	160.0
279.90	261.0
281.10	16592.0
282.10	4642.0
283.00	2505.0
284.10	501.0
285.10	220.0

Instrument :
MSVOA_W
ClientSampleId :
BFB101

m/z	Abundance
36.00	2370.0
37.00	13813.0
38.00	11431.0
39.00	4251.0
39.90	320.0
40.80	54.0
43.00	262.0
44.00	1880.0
45.00	2118.0
46.30	287.0
47.00	2743.0
47.90	1625.0
49.00	11828.0
50.00	52584.0
51.00	15929.0
52.00	731.0
53.20	107.0
54.00	61.0
55.00	791.0
56.00	4316.0
57.00	8213.0
58.00	246.0
59.00	177.0
60.00	2652.0
61.00	13689.0
62.00	12669.0
63.00	10204.0
64.10	963.0
65.10	661.0
65.90	95.0
67.00	631.0
68.00	26240.0
69.00	28448.0
70.00	2331.0
71.20	69.0
72.00	1511.0
73.00	13049.0
74.00	46064.0
75.00	136256.0
76.00	11687.0
77.00	1737.0
78.00	996.0
78.90	8570.0
80.00	2350.0
80.90	8885.0
81.90	1559.0
83.10	255.0
86.10	383.0
87.00	11442.0
88.00	10009.0
90.00	58.0
90.90	1091.0
92.00	7755.0
93.00	11284.0
94.00	32120.0
95.00	255168.0
96.00	17808.0
97.00	704.0
102.90	251.0
103.90	1032.0
104.90	378.0
105.90	1027.0
106.80	241.0
109.90	286.0
110.90	305.0
111.90	213.0
112.90	231.0
115.00	381.0
115.90	834.0
116.90	1485.0
117.90	878.0
119.00	1822.0
119.90	55.0
120.70	101.0
122.70	63.0
123.90	142.0
125.10	463.0
125.70	136.0
126.10	213.0
126.80	67.0
127.90	853.0
128.90	386.0
129.90	748.0
130.90	383.0
133.00	1460.0
134.90	470.0
136.70	311.0
138.70	126.0
139.80	238.0
140.90	2392.0
142.10	350.0

Instrument :
MSVOA_W
ClientSampleId :
BFB101

141.90	201.0
143.00	1540.0
144.10	66.0
144.90	363.0
145.90	320.0
146.90	469.0
147.90	403.0
149.00	270.0
149.90	183.0
152.00	86.0
152.80	102.0
154.10	64.0
154.90	305.0
156.00	103.0
156.70	227.0
157.10	232.0
157.90	89.0
158.90	168.0
160.90	269.0
161.90	67.0
163.00	450.0
163.90	101.0
164.90	446.0
166.00	71.0
169.00	97.0
171.00	126.0
171.90	887.0
174.00	117304.0
174.90	9596.0
176.00	110000.0
177.00	8320.0
178.00	407.0
179.00	714.0
180.00	173.0
188.70	140.0
189.20	201.0
189.80	105.0
191.00	2360.0
191.90	611.0
193.00	2832.0
193.90	617.0
194.90	311.0
203.00	392.0
203.70	79.0
204.20	51.0
204.90	487.0
206.10	101.0
207.00	1930.0
208.00	286.0
209.00	174.0
210.10	83.0
220.80	102.0
235.10	297.0
246.90	98.0
248.90	1311.0
250.00	383.0
251.10	708.0
252.00	163.0
252.80	140.0
265.00	2031.0
266.00	298.0
267.10	334.0
267.80	92.0
278.20	119.0
279.10	170.0
279.80	280.0
281.10	21344.0
282.00	6037.0
283.10	4633.0
283.90	791.0
284.80	148.0
285.40	60.0

Instrument :
MSVOA_W
ClientSampleId :
BFB101

m/z	Abundance
36.00	2621.0
37.00	13719.0
38.00	12379.0
39.10	4726.0
39.90	255.0
41.00	68.0
43.00	298.0
44.00	2094.0
45.00	2706.0
46.00	336.0
47.10	3008.0
48.00	1932.0
49.00	11908.0
50.00	54360.0
51.00	16976.0
52.00	692.0
52.90	183.0
55.00	729.0
56.00	4122.0
57.00	8281.0
58.10	390.0
58.90	334.0
60.00	2860.0
61.00	14291.0
62.00	13741.0
63.00	10219.0
64.00	880.0
65.10	762.0
66.20	108.0
67.00	744.0
68.00	28296.0
69.00	29072.0
70.00	2176.0
70.80	155.0
71.10	147.0
71.90	1723.0
73.00	14287.0
74.00	47872.0
75.00	137088.0
76.00	12371.0
77.10	1534.0
77.90	1255.0
78.90	8969.0
79.90	2422.0
80.90	9173.0
81.90	1906.0
82.90	345.0
85.70	271.0
86.00	260.0
86.90	10984.0
88.00	10274.0
90.00	52.0
90.90	1061.0
92.00	8211.0
93.00	10996.0
94.00	30632.0
95.00	261824.0
96.00	16824.0
97.00	632.0
103.10	530.0
103.90	1295.0
105.10	469.0
105.90	1223.0
107.00	299.0
109.80	212.0
110.30	184.0
111.00	244.0
111.80	217.0
112.00	216.0
112.80	250.0
115.00	449.0
116.00	814.0
116.90	1895.0
118.00	1208.0
118.90	1583.0
119.90	82.0
120.80	102.0
121.90	63.0
122.70	101.0
124.10	225.0
125.10	1031.0
125.80	378.0
126.70	89.0
127.80	887.0
128.90	492.0
129.90	767.0
130.90	356.0
132.00	61.0
133.00	2013.0
134.00	368.0
134.90	759.0

Instrument :
MSVOA_W
ClientSampleId :
BFB101

m/z	Abundance
36.00	1941.0
37.00	10314.0
38.00	9355.0
39.00	3839.0
40.00	237.0
40.90	207.0
43.00	367.0
44.00	1760.0
45.00	2259.0
46.30	247.0
47.10	2211.0
48.00	1364.0
49.00	8916.0
50.00	39384.0
51.00	11910.0
52.00	500.0
52.80	95.0
55.00	557.0
56.00	3332.0
57.00	6064.0
58.00	378.0
59.10	679.0
60.00	2398.0
61.00	10355.0
62.00	9702.0
63.00	8028.0
64.10	966.0
65.10	781.0
66.10	120.0
67.00	517.0
68.00	19976.0
69.00	21640.0
70.00	1801.0
71.00	160.0
72.00	1016.0
73.00	12281.0
74.00	32824.0
75.00	100584.0
76.00	9652.0
77.00	1263.0
78.00	597.0
78.90	6462.0
80.00	1804.0
80.90	6542.0
81.90	1501.0
83.10	241.0
83.60	128.0
84.90	78.0
85.70	172.0
87.00	8276.0
87.90	7517.0
89.10	186.0
90.90	783.0
92.00	5371.0
93.00	7934.0
94.00	22056.0
95.00	177600.0
96.00	12900.0
97.10	462.0
98.20	66.0
103.00	710.0
103.90	912.0
104.90	371.0
106.00	844.0
107.00	122.0
109.80	339.0
110.90	362.0
111.90	327.0
112.90	202.0
114.90	384.0
115.90	754.0
117.00	1228.0
117.80	975.0
119.00	1342.0
119.90	96.0
120.90	135.0
121.90	59.0
123.70	98.0
125.10	898.0
125.90	263.0
127.90	688.0
128.90	328.0
129.90	548.0
130.80	232.0
131.80	90.0
133.00	2801.0
135.00	574.0
136.00	52.0
136.90	212.0
138.60	57.0
141.00	1278.0

Instrument :
MSVOA_W
ClientSampleId :
BFB101