

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060324\
 Data File : VW028978.D
 Acq On : 03 Jun 2024 21:05
 Operator : SY/MD
 Sample : P2678-21
 Misc : 5.68g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 04 02:22:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 04 02:14:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	465444	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	364127	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	109165	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	165810	22.424	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.680%
7) Chloroethane-d5	2.899	69	128708	22.668	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.680%
11) 1,1-Dichloroethene-d2	4.021	65	68809	21.172	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.680%
21) 2-Butanone-d5	7.075	46	68423	45.291	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.580%
24) Chloroform-d	7.648	84	293460	22.100	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.400%
26) 1,2-Dichloroethane-d4	8.307	65	161165	23.054	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.200%
32) Benzene-d6	8.276	84	578182	25.870	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.480%
36) 1,2-Dichloropropane-d6	9.270	67	183587	27.093	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.360%
41) Toluene-d8	10.325	98	471696	23.651	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.600%
43) trans-1,3-Dichloroprop...	10.575	79	53586	20.580	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.320%
47) 2-Hexanone-d5	10.922	63	43991	49.195	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.400%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	120072	25.507	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.040%
66) 1,2-Dichlorobenzene-d4	13.848	152	98748	25.491	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.960%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3981	0.462	ug/L	# 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060324\
Data File : VW028978.D
Acq On : 03 Jun 2024 21:05
Operator : SY/MD
Sample : P2678-21
Misc : 5.68g/10mL/MSVOA_W/SOIL/A
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 04 02:22:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 04 02:14:06 2024
Response via : Initial Calibration

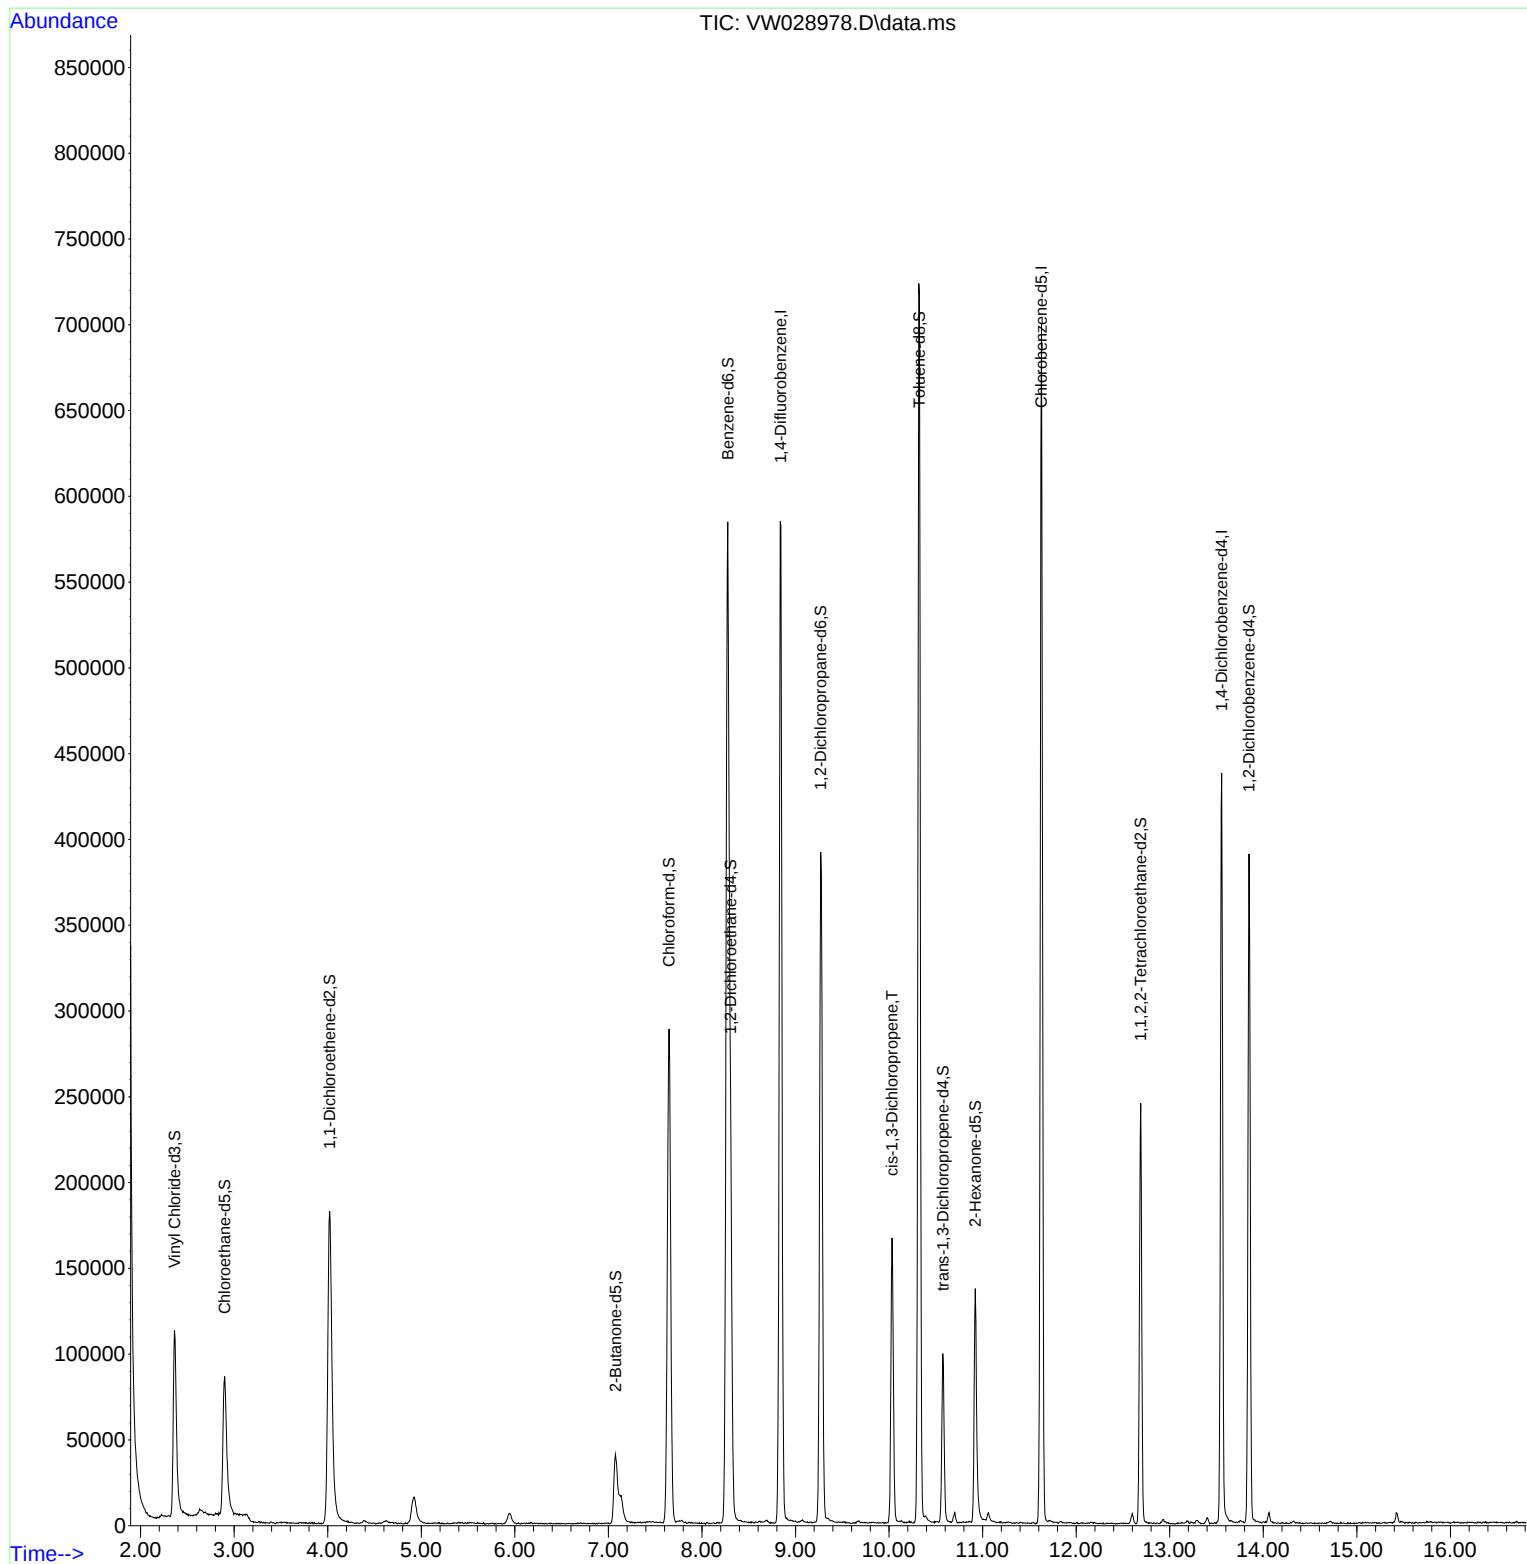

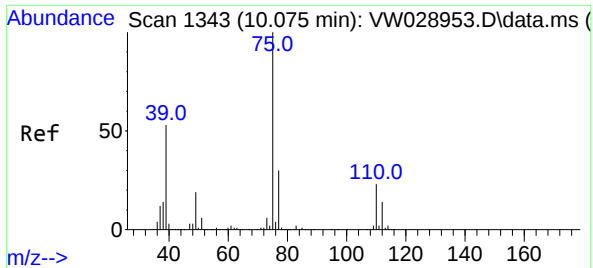

#39
 cis-1,3-Dichloropropene
 Concen: 0.462 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW028978.D
 Acq: 03 Jun 2024 21:05

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3981
 Ion Ratio Lower Upper
 75 100
 77 52.2 21.0 39.0#

