




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060324\
 Data File : VW028964.D
 Acq On : 03 Jun 2024 15:30
 Operator : SY/MD
 Sample : P2678-07
 Misc : 6.26g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH676

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/04/2024
 Supervised By :Mahesh Dadoda 06/04/2024

Quant Time: Jun 04 02:20:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 04 02:14:06 2024
 Response via : Initial Calibration

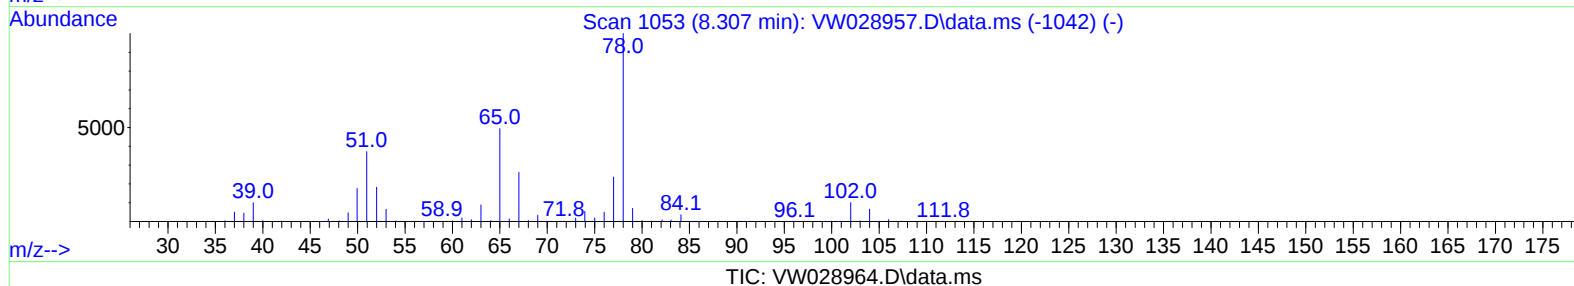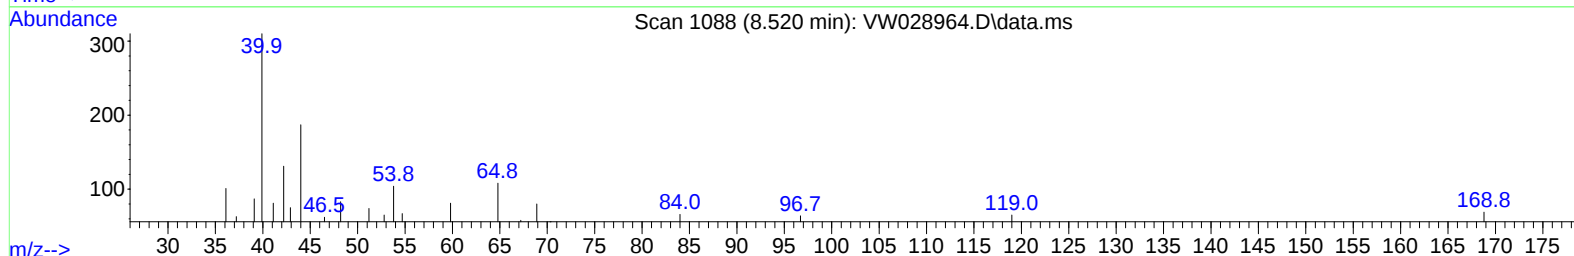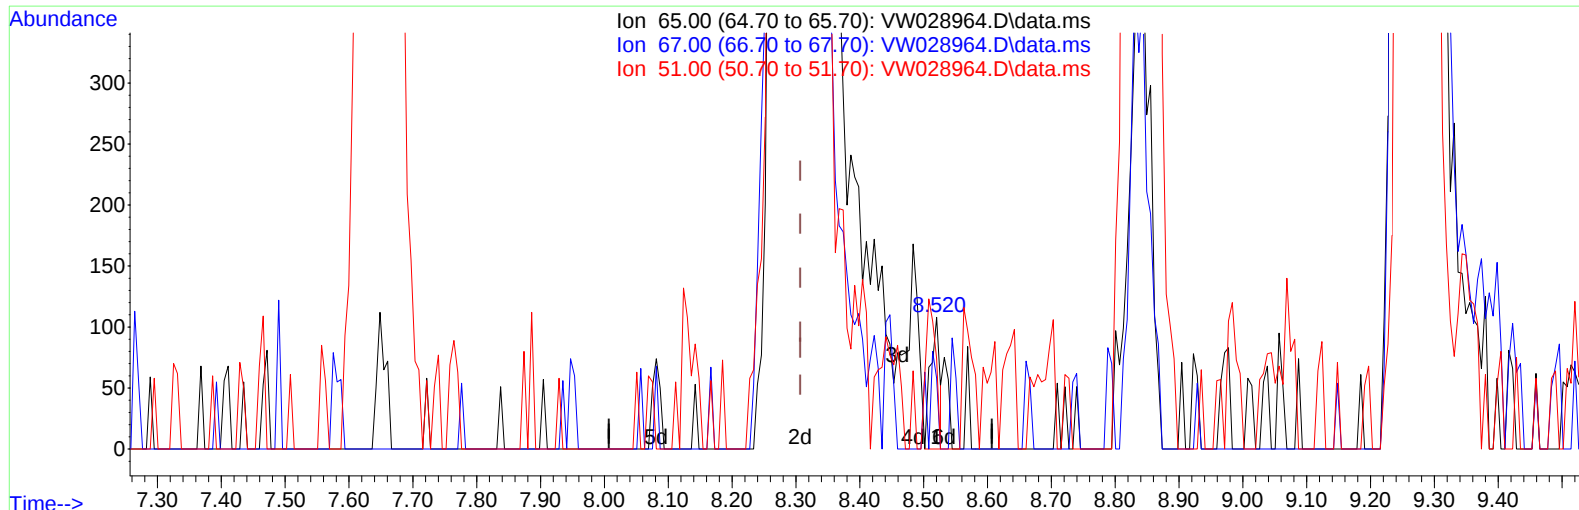

(26) 1,2-Dichloroethane-d4 (S)

8.520min (+ 0.213) 0.01 ug/L

response 109

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	45.87
51.00	105.10	122.02
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060324\
 Data File : VW028964.D
 Acq On : 03 Jun 2024 15:30
 Operator : SY/MD
 Sample : P2678-07
 Misc : 6.26g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH676

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/04/2024
 Supervised By :Mahesh Dadoda 06/04/2024

Quant Time: Jun 04 02:20:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 04 02:14:06 2024
 Response via : Initial Calibration

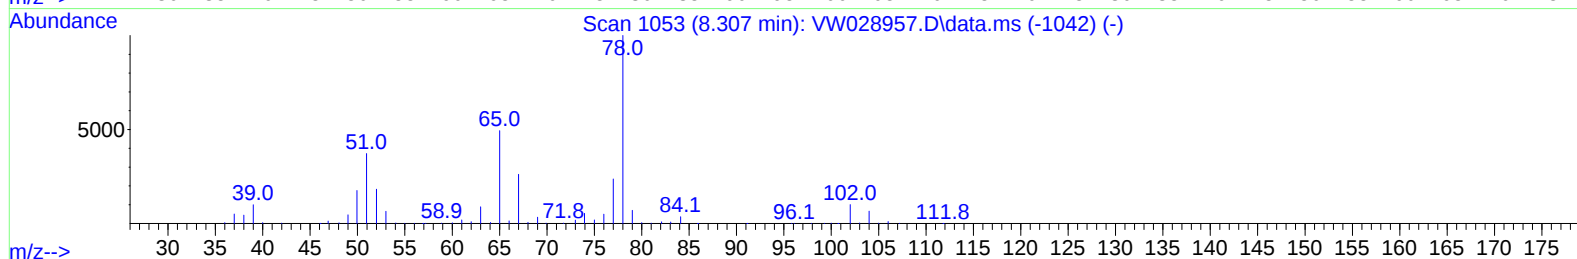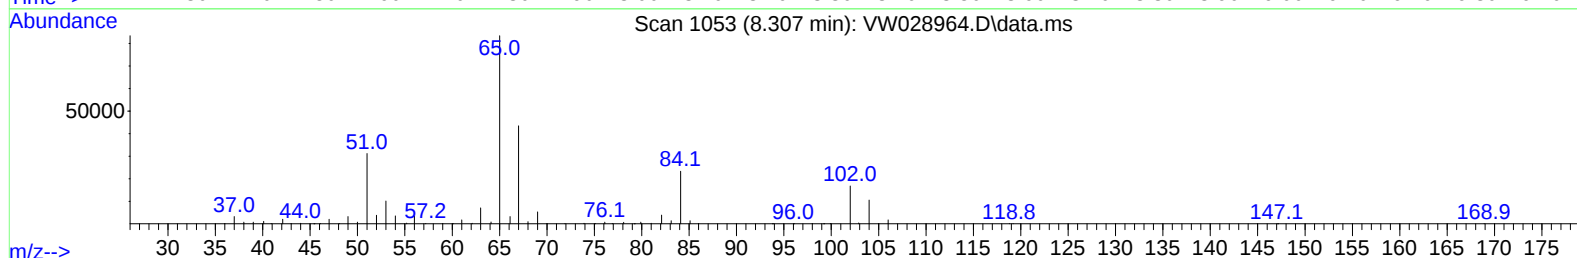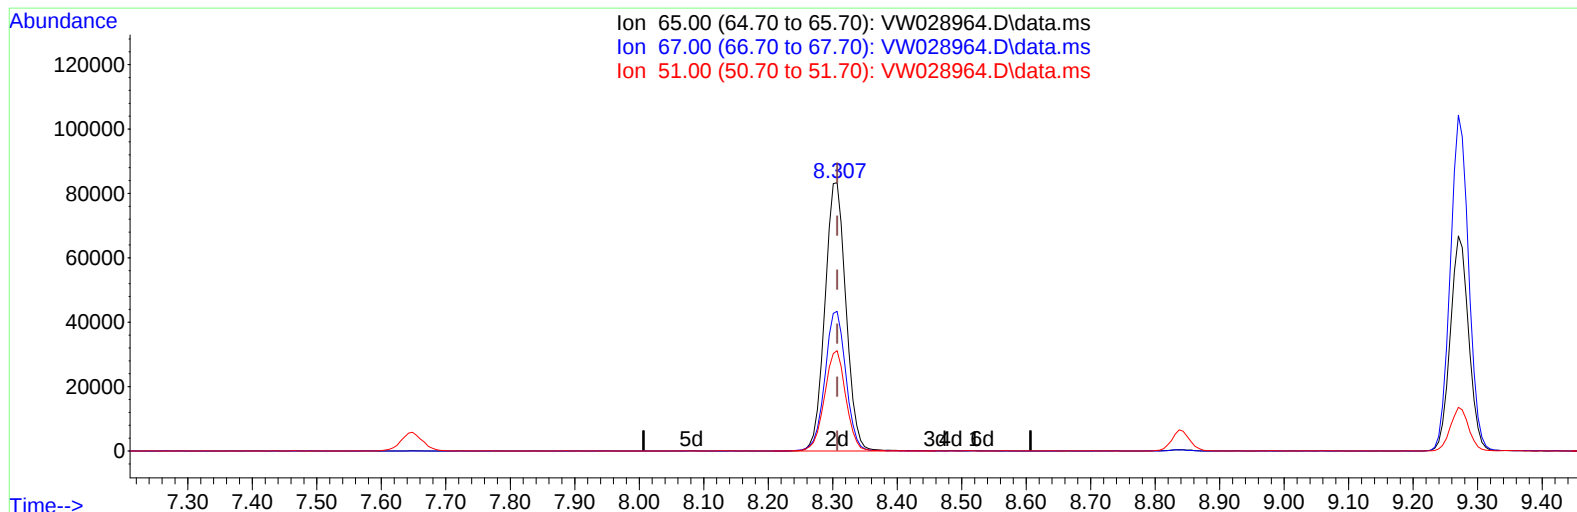

TIC: VW028964.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 21.22 ug/L m

response 189465

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.03#
51.00	105.10	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060324\
 Data File : VW028964.D
 Acq On : 03 Jun 2024 15:30
 Operator : SY/MD
 Sample : P2678-07
 Misc : 6.26g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH676

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/04/2024
 Supervised By :Mahesh Dadoda 06/04/2024

Quant Time: Jun 04 02:20:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 04 02:14:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	594432	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	520228	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	220944	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	179244	18.981	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.920%
7) Chloroethane-d5	2.893	69	137735	18.994	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.960%
11) 1,1-Dichloroethene-d2	4.021	65	79252	19.094	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.360%
21) 2-Butanone-d5	7.075	46	87519	45.360	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.720%
24) Chloroform-d	7.648	84	329441	19.426	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.720%
26) 1,2-Dichloroethane-d4	8.307	65	189465m	21.221	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.880%
32) Benzene-d6	8.270	84	679692	21.287	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.160%
36) 1,2-Dichloropropane-d6	9.270	67	206812	21.362	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.440%
41) Toluene-d8	10.319	98	597207	20.959	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.840%
43) trans-1,3-Dichloroprop...	10.575	79	78150	21.008	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.040%
47) 2-Hexanone-d5	10.922	63	61739	48.326	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.660%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	148693	22.109	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.440%
66) 1,2-Dichlorobenzene-d4	13.849	152	172918	22.055	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.200%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060324\
Data File : VW028964.D
Acq On : 03 Jun 2024 15:30
Operator : SY/MD
Sample : P2678-07
Misc : 6.26g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH676

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/04/2024
Supervised By :Mahesh Dadoda 06/04/2024

Quant Time: Jun 04 02:20:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 04 02:14:06 2024
Response via : Initial Calibration

