

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060424\
Data File : VW029003.D
Acq On : 04 Jun 2024 18:29
Operator : SY/MD
Sample : P2710-08
Misc : 4.13g/10mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
A4BL7

Manual IntegrationsAPPROVED

Quant Time: Jun 05 00:51:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 05 00:46:16 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

06/05/2024
Supervised By :Mahesh
Dadoda

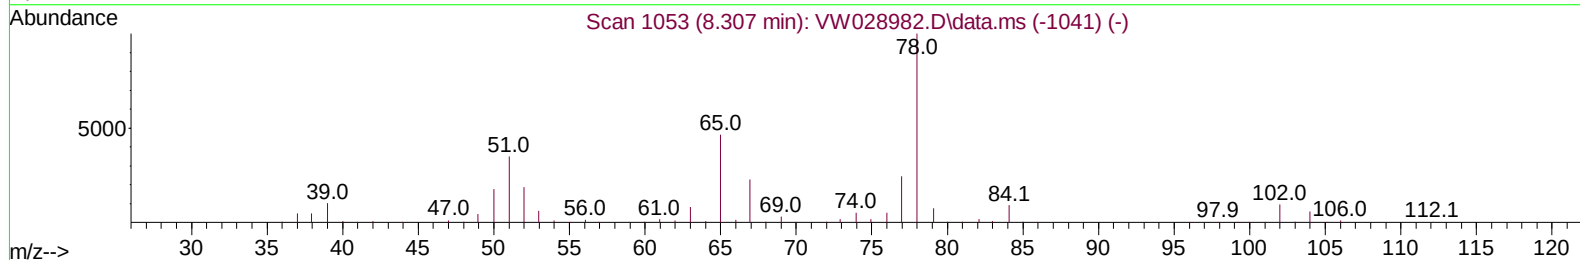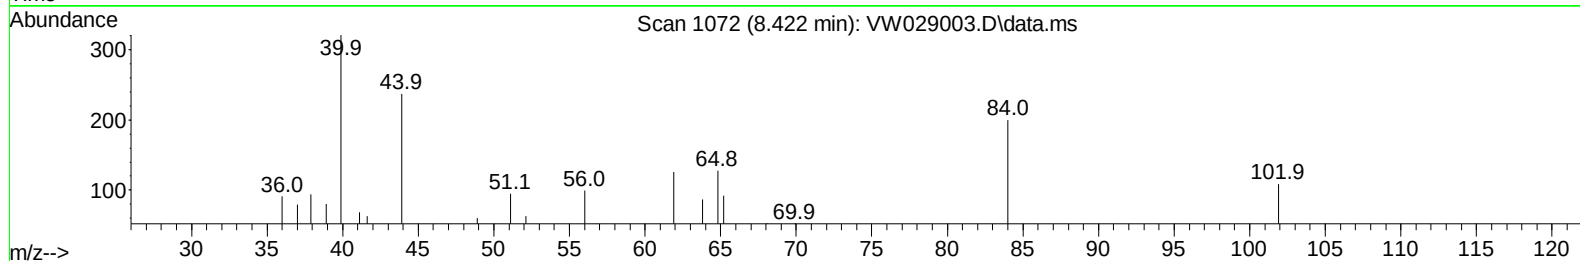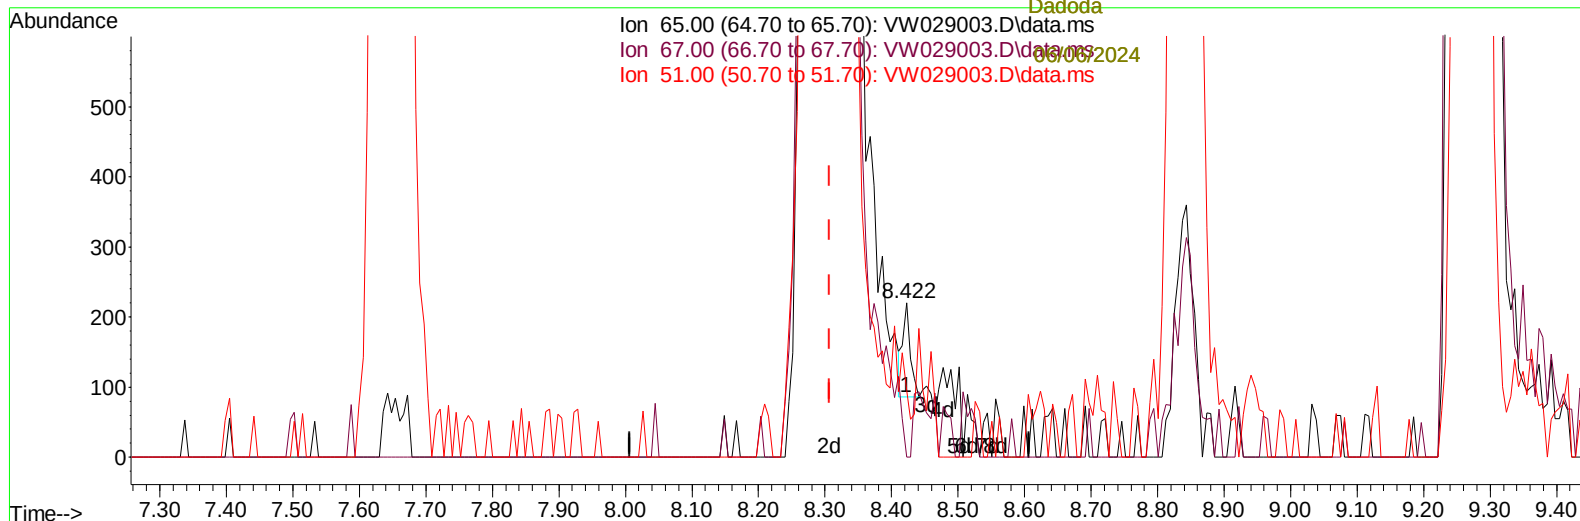

TIC: VW029003.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.422min (+ 0.116) 0.02 ug/L

response 105

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	58.10
51.00	105.10	97.14
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060424\
 Data File : VW029003.D
 Acq On : 04 Jun 2024 18:29
 Operator : SY/MD
 Sample : P2710-08
 Misc : 4.13g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BL7




Manual IntegrationsAPPROVED

Quant Time: Jun 05 00:51:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 05 00:46:16 2024
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

06/05/2024
 Supervised By :Mahesh
 Dadoda

Ion 65.00 (64.70 to 65.70): VW029003.D\data.ms
 Ion 67.00 (66.70 to 67.70): VW029003.D\data.ms
 Ion 51.00 (50.70 to 51.70): VW029003.D\data.ms

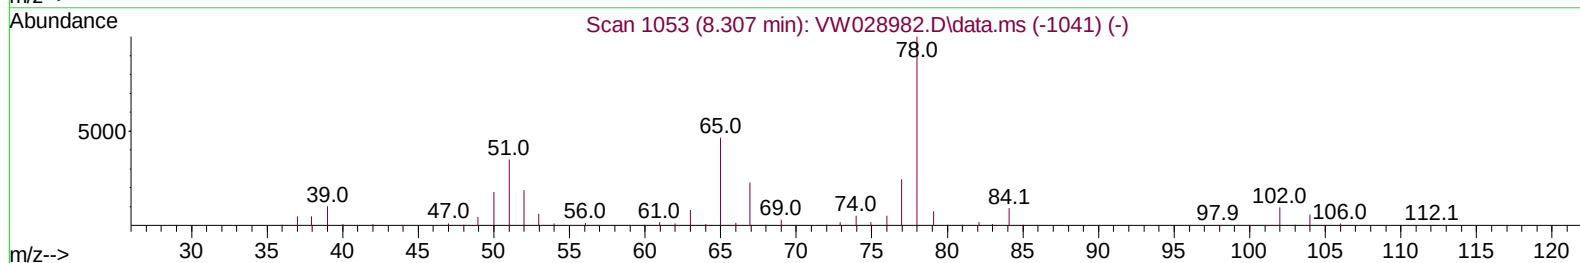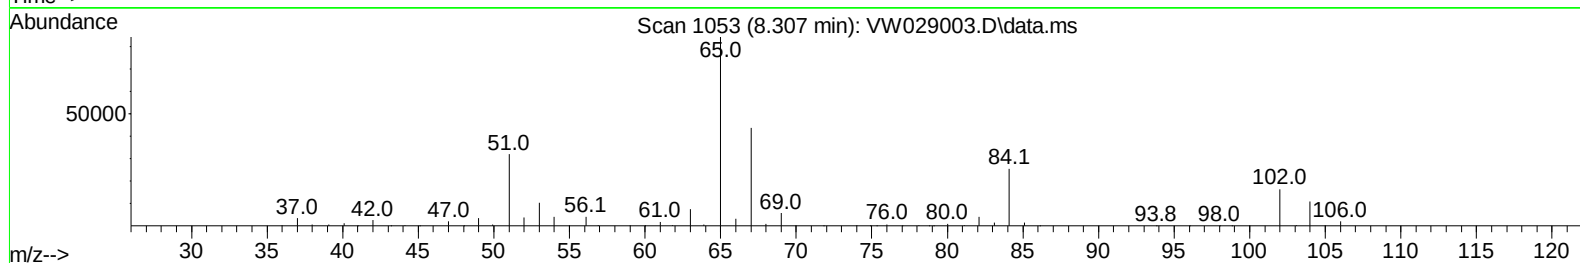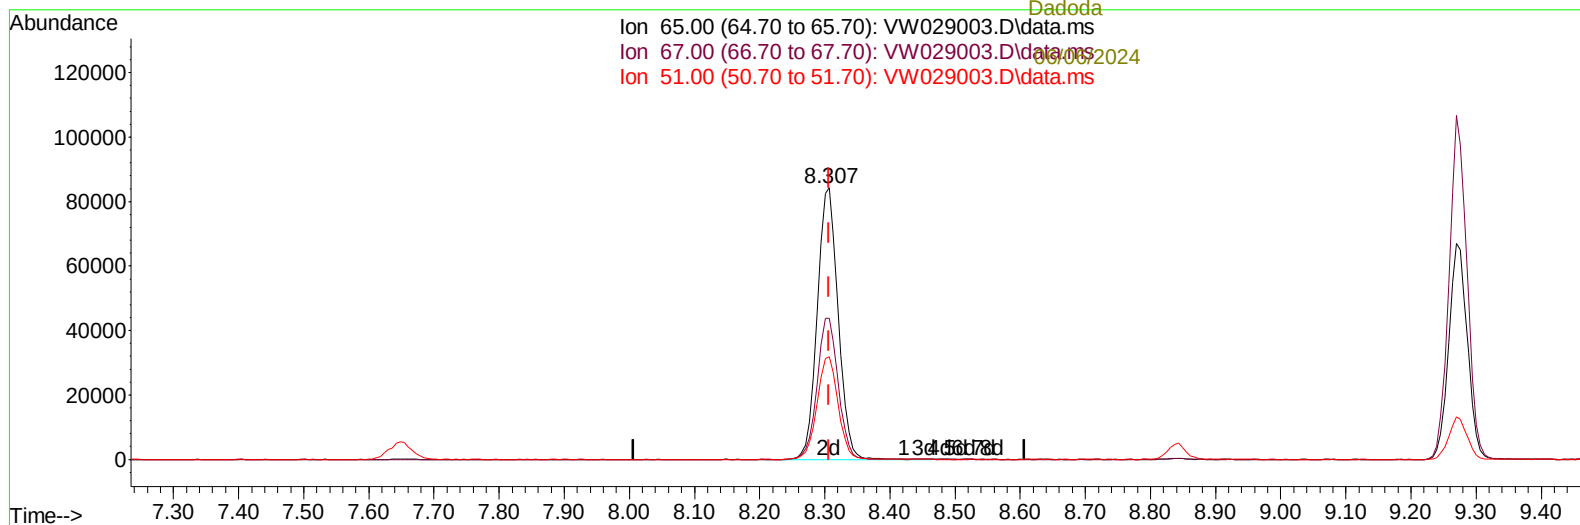

TIC: VW029003.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 28.49 ug/L m

response 187478

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.03#
51.00	105.10	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060424\
 Data File : VW029003.D
 Acq On : 04 Jun 2024 18:29
 Operator : SY/MD
 Sample : P2710-08
 Misc : 4.13g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BL7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

06/05/2024
 Supervised By :Mahesh
 Dadoda

Quant Time: Jun 05 00:51:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 05 00:46:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----06/06/2024						
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	438168	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	291358	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	63019	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	192911	27.714	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	110.840%	
7) Chloroethane-d5	2.899	69	153455	28.709	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	114.840%	
11) 1,1-Dichloroethene-d2	4.021	65	81993	26.800	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	107.200%	
21) 2-Butanone-d5	7.081	46	48513	34.111	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	68.220%	
24) Chloroform-d	7.648	84	327960	26.236	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	104.960%	
26) 1,2-Dichloroethane-d4	8.307	65	187478m	28.487	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	113.960%	
32) Benzene-d6	8.270	84	664553	37.162	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	148.640%#	
36) 1,2-Dichloropropane-d6	9.270	67	205168	37.840	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	151.360%#	
41) Toluene-d8	10.318	98	504787	31.632	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	126.520%	
43) trans-1,3-Dichloroprop...	10.575	79	41691	20.011	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	80.040%	
47) 2-Hexanone-d5	10.922	63	32903	45.985	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.980%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	107029	28.414	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	113.640%	
66) 1,2-Dichlorobenzene-d4	13.848	152	62940	28.145	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	112.560%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060424\
Data File : VW029003.D
Acq On : 04 Jun 2024 18:29
Operator : SY/MD
Sample : P2710-08
Misc : 4.13g/10mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BL7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

06/05/2024
Supervised By :Mahesh
Dadoda

06/06/2024

Quant Time: Jun 05 00:51:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 05 00:46:16 2024
Response via : Initial Calibration

