

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060424\
 Data File : VW028988.D
 Acq On : 04 Jun 2024 12:10
 Operator : SY/MD
 Sample : P2678-18RE
 Misc : 4.72g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH687RE

Quant Time: Jun 05 00:48:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 05 00:46:16 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	305699	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	226195	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	61544	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.357	65	143992	29.650	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	118.600%	
7) Chloroethane-d5		2.899	69	113251	30.368	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	121.480%	
11) 1,1-Dichloroethene-d2		4.021	65	59929	28.076	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	112.320%#	
21) 2-Butanone-d5		7.075	46	52080	52.487	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.980%	
24) Chloroform-d		7.648	84	251709	28.861	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	115.440%	
26) 1,2-Dichloroethane-d4		8.301	65	136826	29.800	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	119.200%	
32) Benzene-d6		8.276	84	498078	35.876	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	143.520%#	
36) 1,2-Dichloropropane-d6		9.270	67	159448	37.879	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	151.520%#	
41) Toluene-d8		10.325	98	382150	30.846	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	123.400%	
43) trans-1,3-Dichloroprop...		10.575	79	45660	28.229	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	112.920%	
47) 2-Hexanone-d5		10.922	63	31493	56.695	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.380%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	88583	30.292	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.160%#	
66) 1,2-Dichlorobenzene-d4		13.848	152	64555	29.559	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	118.240%	
Target Compounds							
13) Acetone		4.125	43	15926	15.316	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060424\
Data File : VW028988.D
Acq On : 04 Jun 2024 12:10
Operator : SY/MD
Sample : P2678-18RE
Misc : 4.72g/10mL/MSVOA_W/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH687RE

Quant Time: Jun 05 00:48:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 05 00:46:16 2024
Response via : Initial Calibration

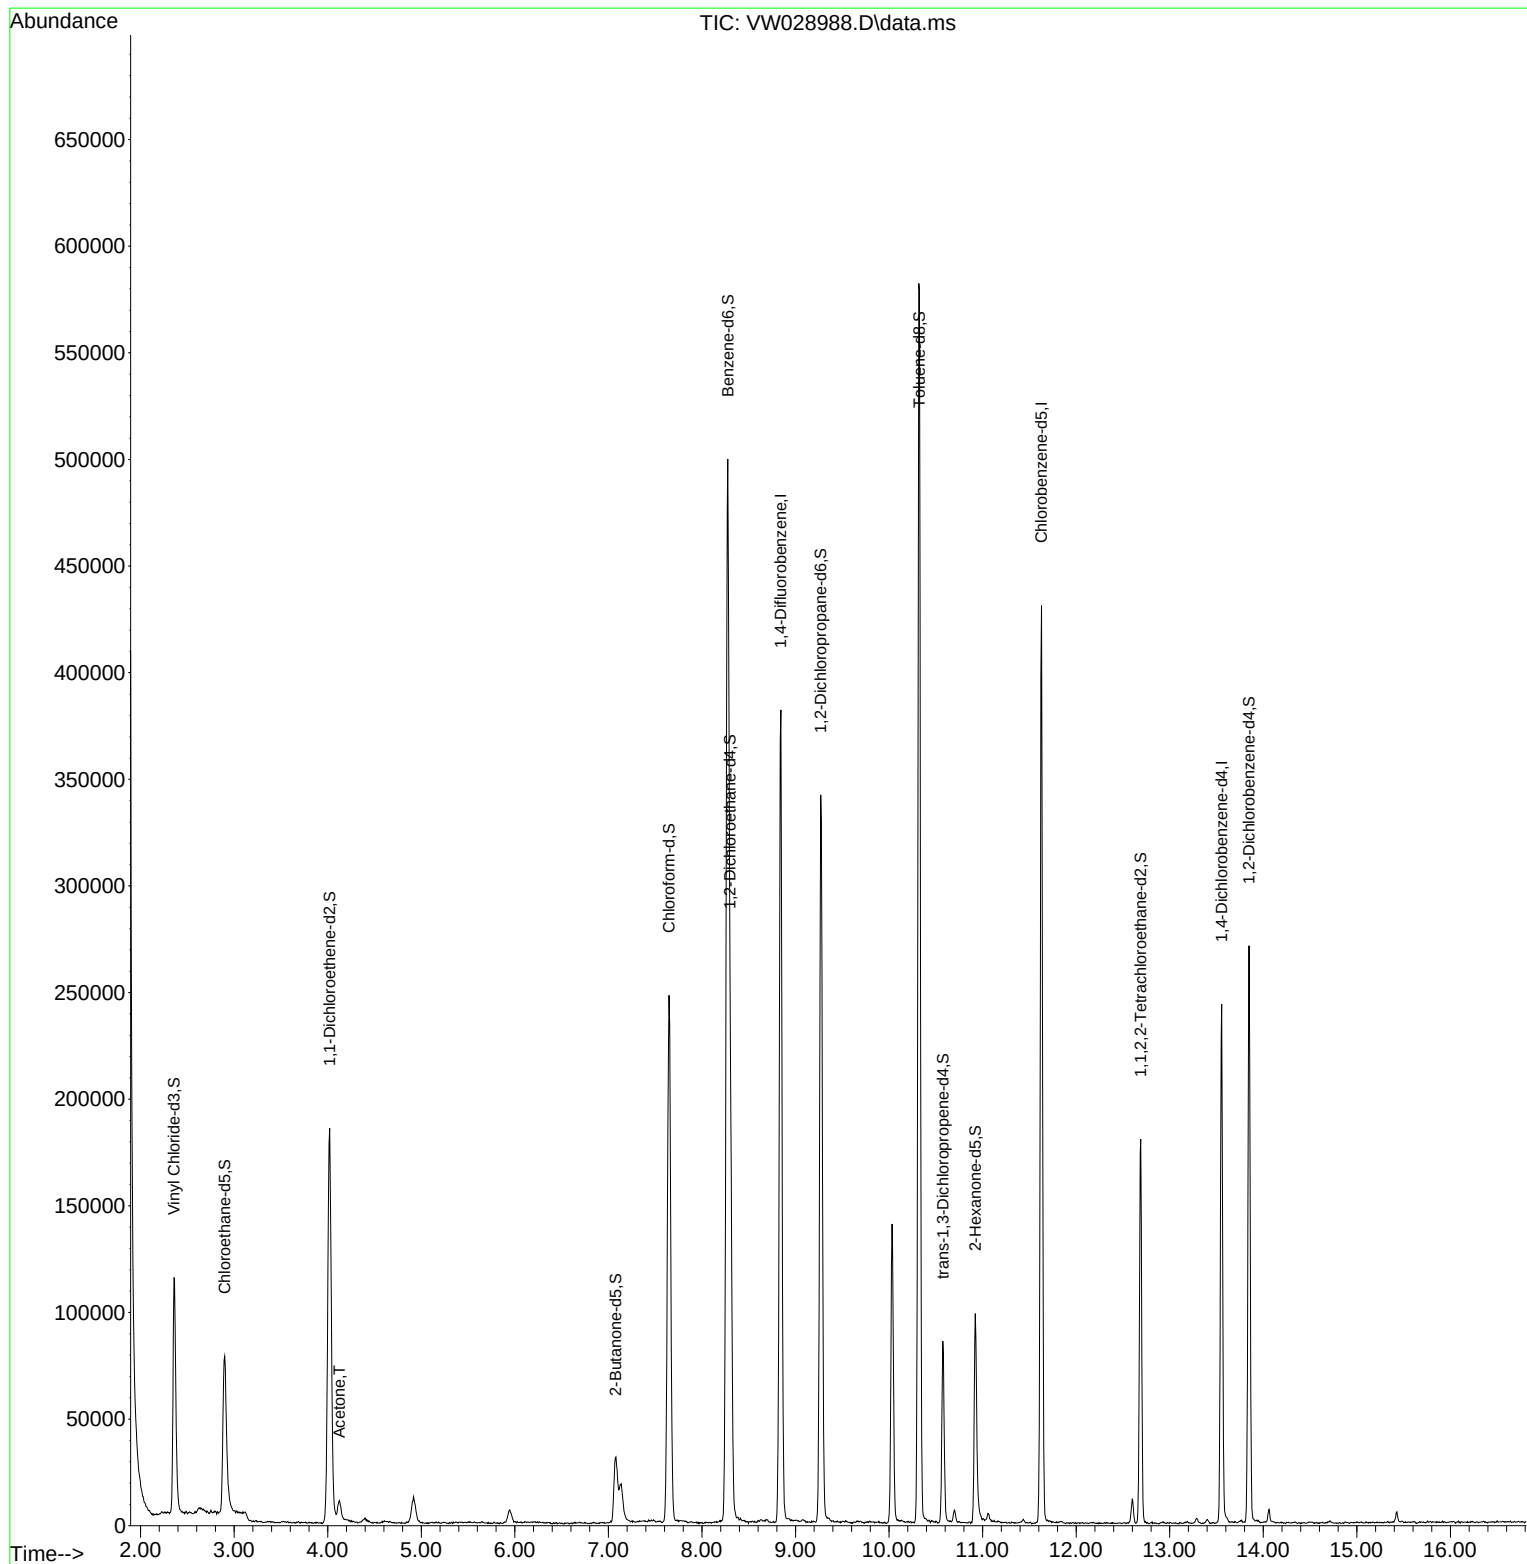

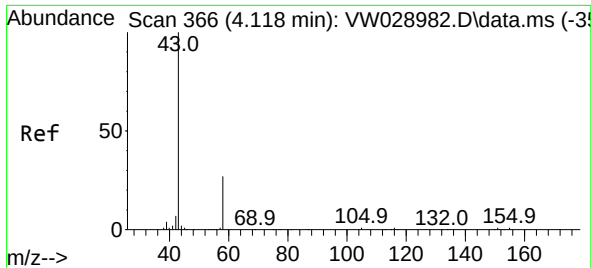

#13
 Acetone
 Concen: 15.316 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW028988.D
 Acq: 04 Jun 2024 12:10

Instrument :
 MSVOA_W
 ClientSampleId :
 BH687RE

Tgt Ion: 43 Resp: 15926
 Ion Ratio Lower Upper
 43 100
 58 30.5 0.0 59.4

