

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060424\
 Data File : VW029001.D
 Acq On : 04 Jun 2024 17:41
 Operator : SY/MD
 Sample : P2710-06
 Misc : 4.82g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4B27

Quant Time: Jun 05 00:51:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 05 00:46:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	501801	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	392093	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	114921	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	182259	22.863	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.440%
7) Chloroethane-d5	2.899	69	145646	23.792	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.160%
11) 1,1-Dichloroethene-d2	4.021	65	78392	22.373	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.480%
21) 2-Butanone-d5	7.075	46	80332	49.321	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.640%
24) Chloroform-d	7.648	84	337945	23.606	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.440%
26) 1,2-Dichloroethane-d4	8.307	65	190584	25.287	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.160%
32) Benzene-d6	8.270	84	684682	28.451	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	113.800%
36) 1,2-Dichloropropane-d6	9.270	67	212864	29.173	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	116.680%
41) Toluene-d8	10.325	98	565333	26.324	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.280%
43) trans-1,3-Dichloroprop...	10.575	79	63897	22.790	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.160%
47) 2-Hexanone-d5	10.922	63	55432	57.568	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.140%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	132326	26.105	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.400%
66) 1,2-Dichlorobenzene-d4	13.848	152	101014	24.770	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.080%
Target Compounds						
					Qvalue	
13) Acetone	4.125	43	19471	11.407	ug/L	100
16) Methylene chloride	4.923	84	26333	3.497	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060424\
Data File : VW029001.D
Acq On : 04 Jun 2024 17:41
Operator : SY/MD
Sample : P2710-06
Misc : 4.82g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4B27

Quant Time: Jun 05 00:51:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 05 00:46:16 2024
Response via : Initial Calibration




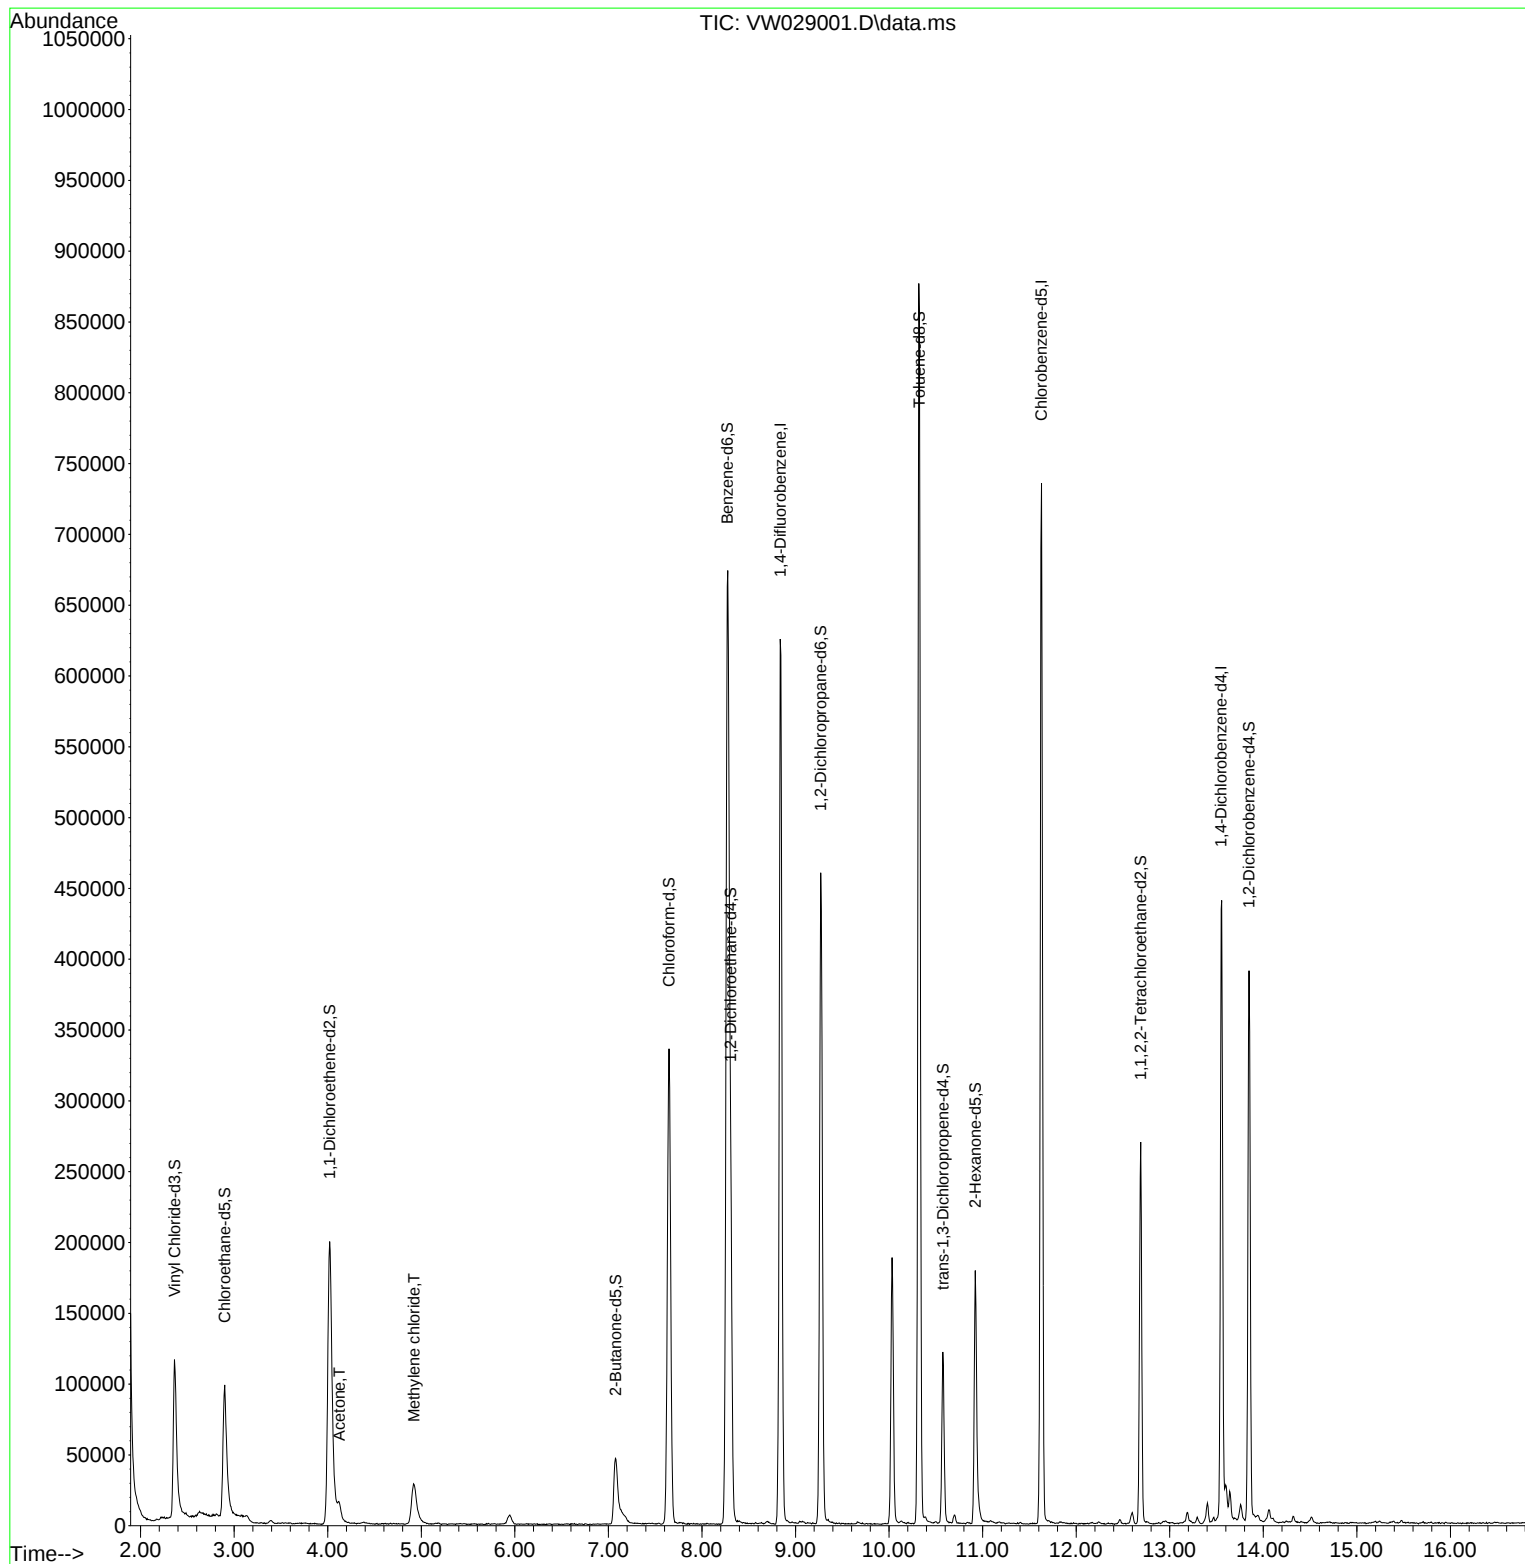


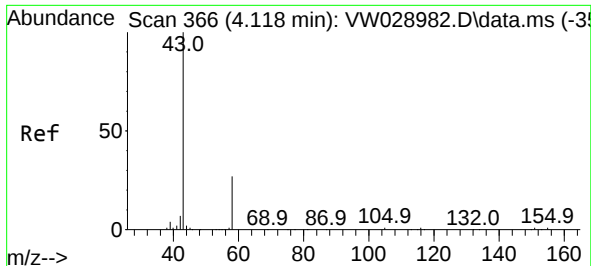

#13
Acetone
Concen: 11.407 ug/L
RT: 4.125 min Scan# 367
Delta R.T. 0.006 min
Lab File: VW029001.D
Acq: 04 Jun 2024 17:41

Instrument :
MSVOA_W
ClientSampleId :
A4B27

Tgt Ion: 43 Resp: 19471
Ion Ratio Lower Upper
43 100
58 29.9 0.0 59.4

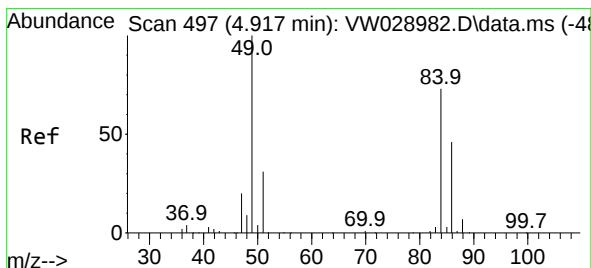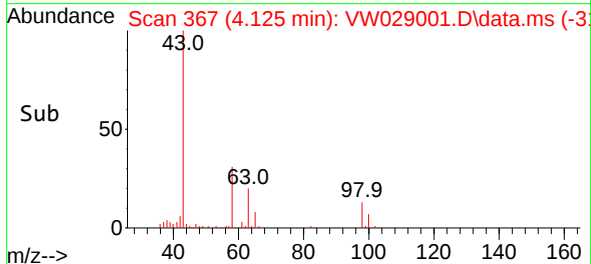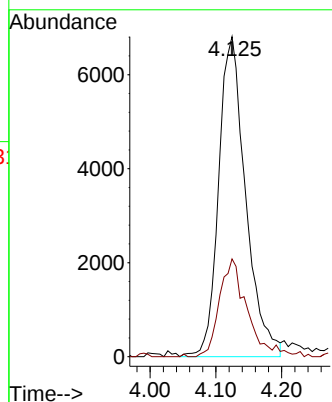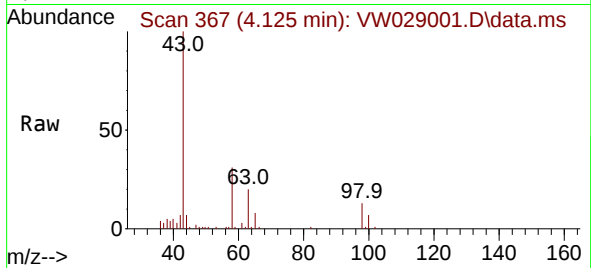

#16
Methylene chloride
Concen: 3.497 ug/L
RT: 4.923 min Scan# 498
Delta R.T. 0.006 min
Lab File: VW029001.D
Acq: 04 Jun 2024 17:41

Tgt Ion: 84 Resp: 26333
Ion Ratio Lower Upper
84 100
86 53.2 43.8 81.4
49 123.7 91.3 169.5

