

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060524\
 Data File : VW029013.D
 Acq On : 05 Jun 2024 11:33
 Operator : SY/MD
 Sample : P2710-11
 Misc : 4.20g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 05 23:51:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 05 23:49:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	560746	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	414135	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	115911	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	218351	24.511	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.040%
7) Chloroethane-d5	2.899	69	175207	25.613	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.440%
11) 1,1-Dichloroethene-d2	4.021	65	96808	24.725	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	98.920%
21) 2-Butanone-d5	7.075	46	75482	41.472	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.940%
24) Chloroform-d	7.648	84	401296	25.085	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.320%
26) 1,2-Dichloroethane-d4	8.307	65	218217	25.910	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.640%
32) Benzene-d6	8.270	84	816476	32.121	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	128.480%
36) 1,2-Dichloropropane-d6	9.270	67	251698	32.659	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	130.640%#
41) Toluene-d8	10.325	98	677428	29.865	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	119.480%
43) trans-1,3-Dichloroprop...	10.575	79	77600	26.204	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	104.800%
47) 2-Hexanone-d5	10.922	63	52459	51.581	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.160%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	138715	25.909	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.640%
66) 1,2-Dichlorobenzene-d4	13.848	152	108886	26.472	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.880%
Target Compounds					Qvalue	
48) 2-Hexanone	10.922	43	8667	3.370	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060524\
Data File : VW029013.D
Acq On : 05 Jun 2024 11:33
Operator : SY/MD
Sample : P2710-11
Misc : 4.20g/10mL/MSVOA_W/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jun 05 23:51:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 05 23:49:22 2024
Response via : Initial Calibration

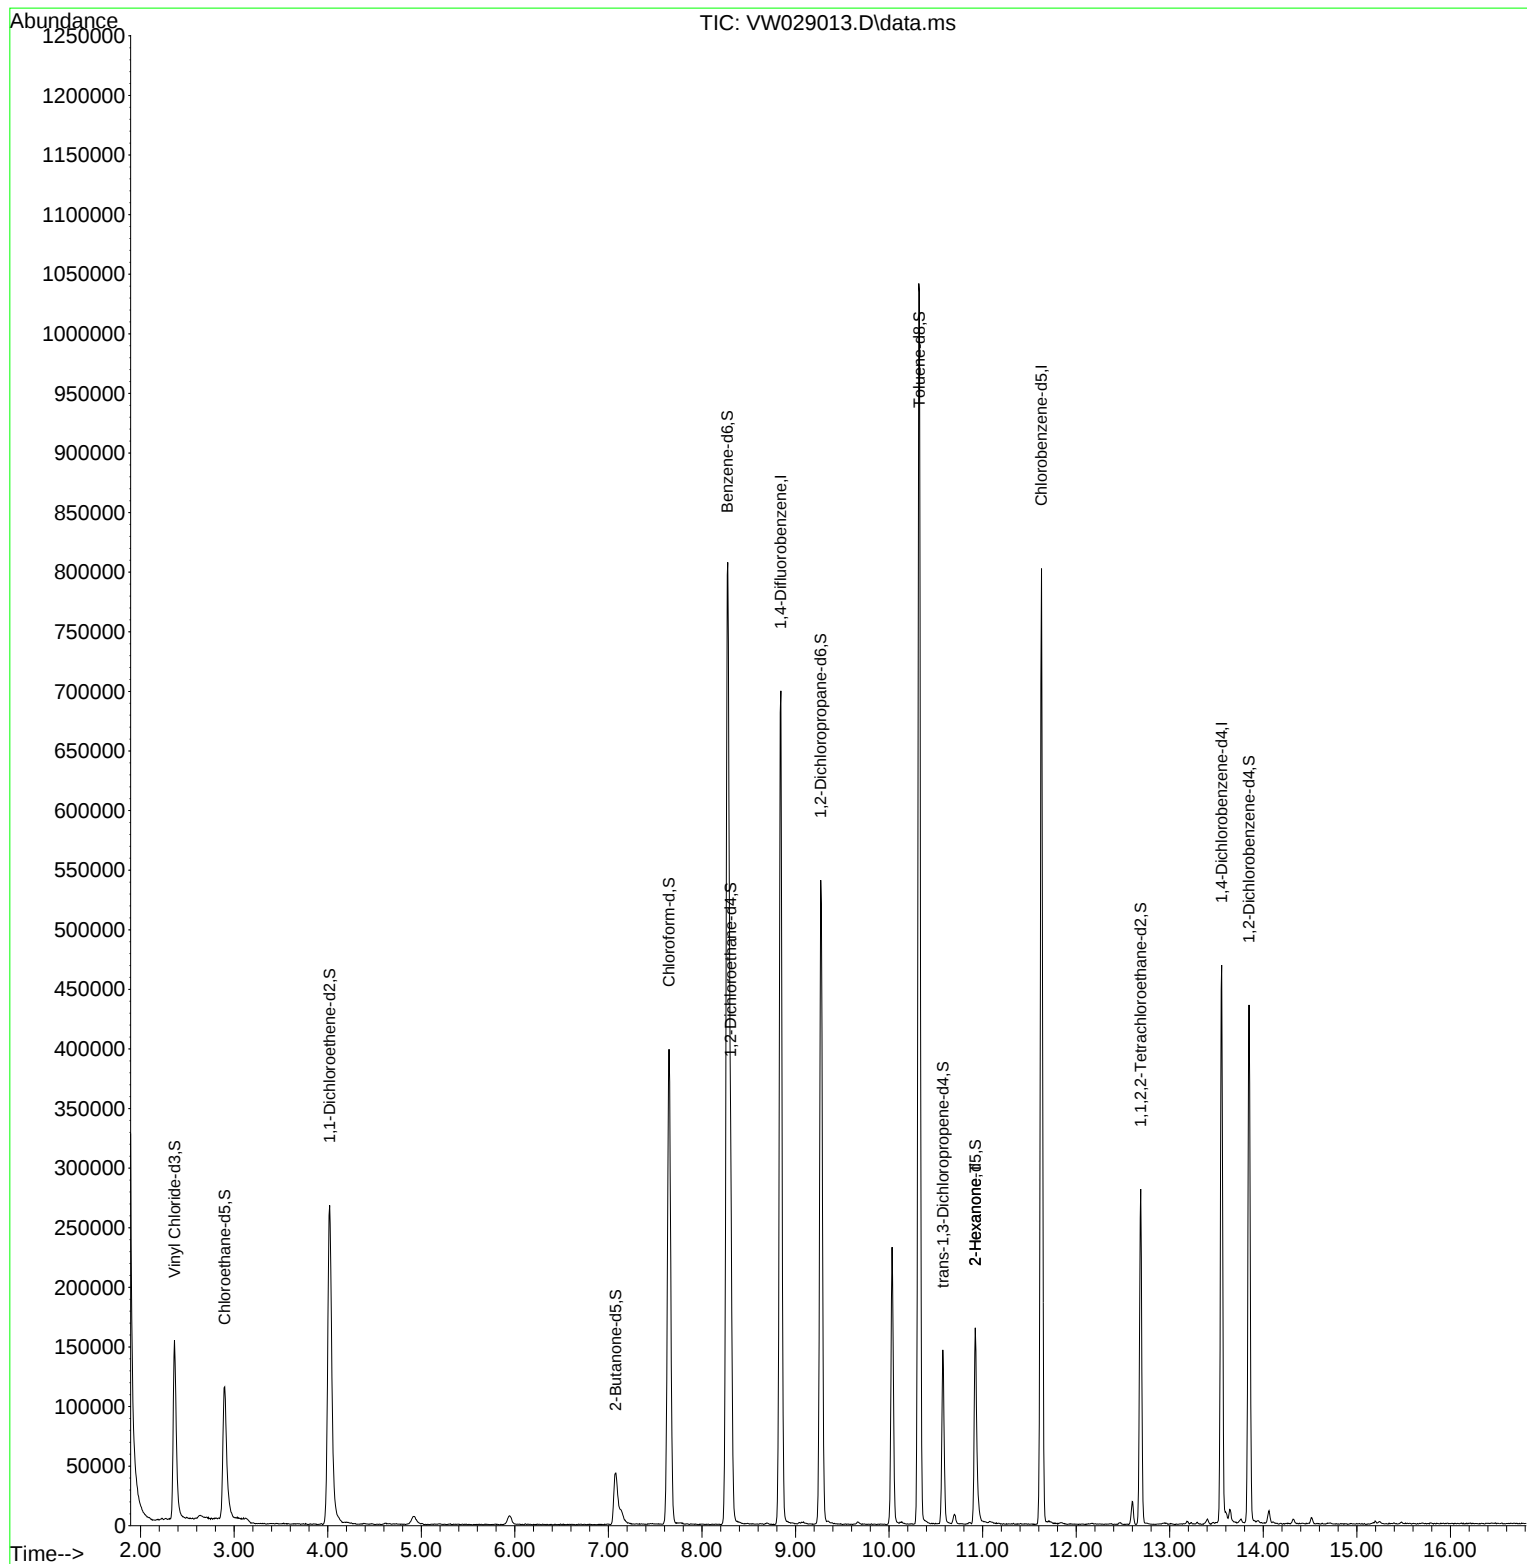

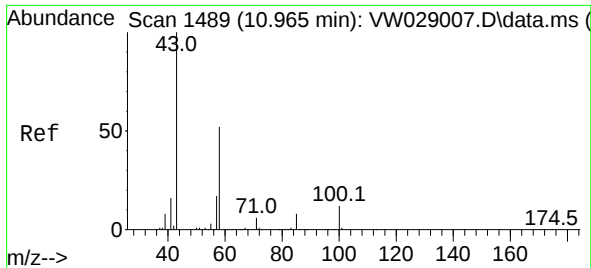

#48
 2-Hexanone
 Concen: 3.370 ug/L
 RT: 10.922 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW029013.D
 Acq: 05 Jun 2024 11:33

Instrument :
 MSVOA_W
 ClientSampleId :

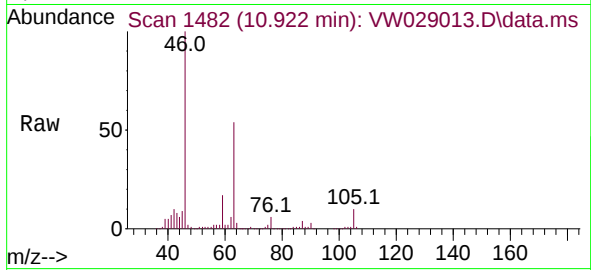

Tgt Ion: 43 Resp: 8667

Ion	Ratio	Lower	Upper
43	100		
58	22.0	41.4	62.0#
57	27.9	14.2	21.4#
100	1.4	9.1	13.7#

