




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060524\
 Data File : VW029012.D
 Acq On : 05 Jun 2024 11:09
 Operator : SY/MD
 Sample : P2710-10
 Misc : 5.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BL9

Manual IntegrationsAPPROVED

Quant Time: Jun 05 23:50:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 05 23:49:22 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/06/2024
 Supervised By :Mahesh Dadoda 06/06/2024

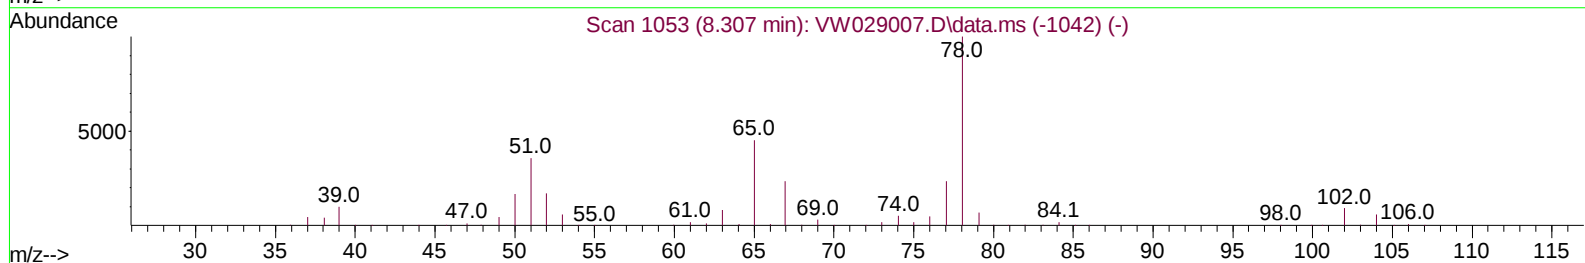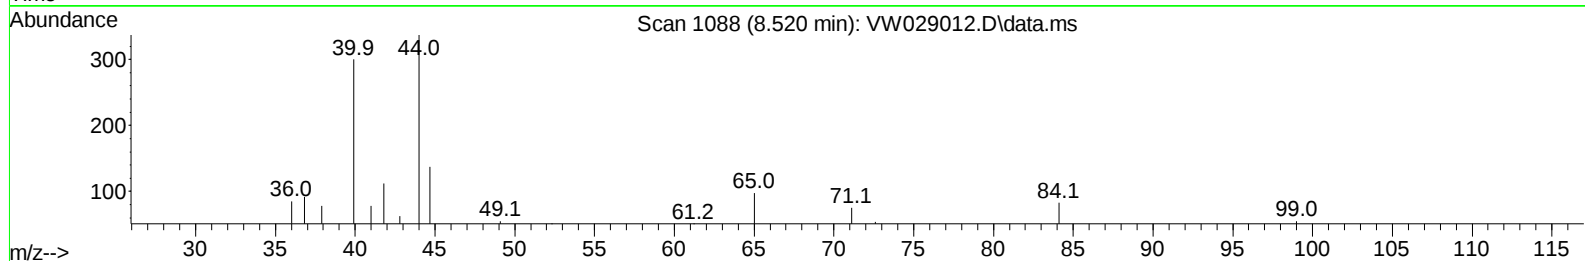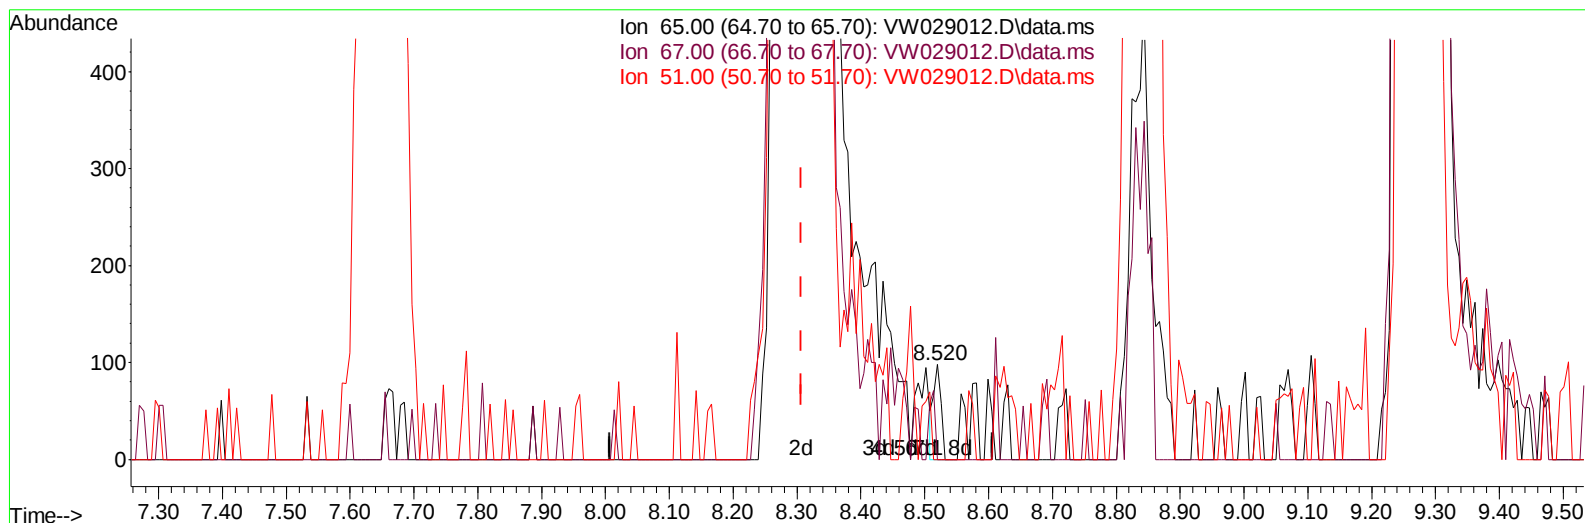

TIC: VW029012.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.520min (+ 0.213) 0.01 ug/L

response 81

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	58.02
51.00	105.10	83.95
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060524\
 Data File : VW029012.D
 Acq On : 05 Jun 2024 11:09
 Operator : SY/MD
 Sample : P2710-10
 Misc : 5.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BL9

Manual IntegrationsAPPROVED

Quant Time: Jun 05 23:50:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 05 23:49:22 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/06/2024
 Supervised By :Mahesh Dadoda 06/06/2024

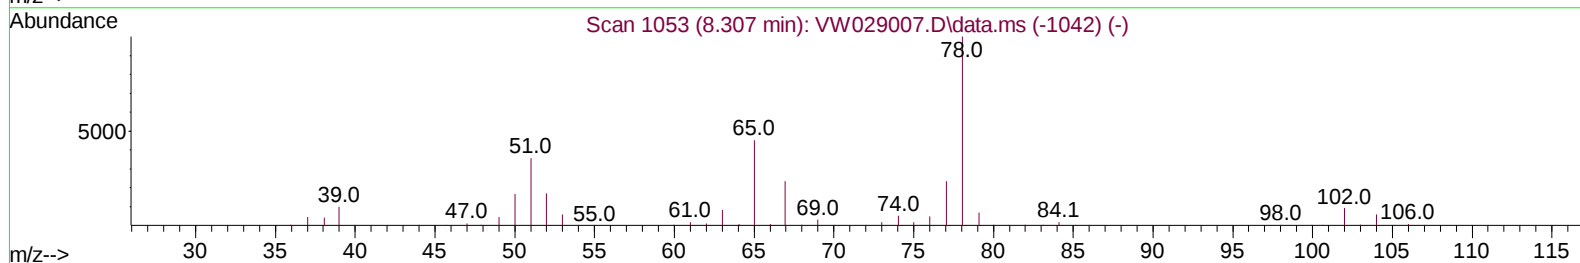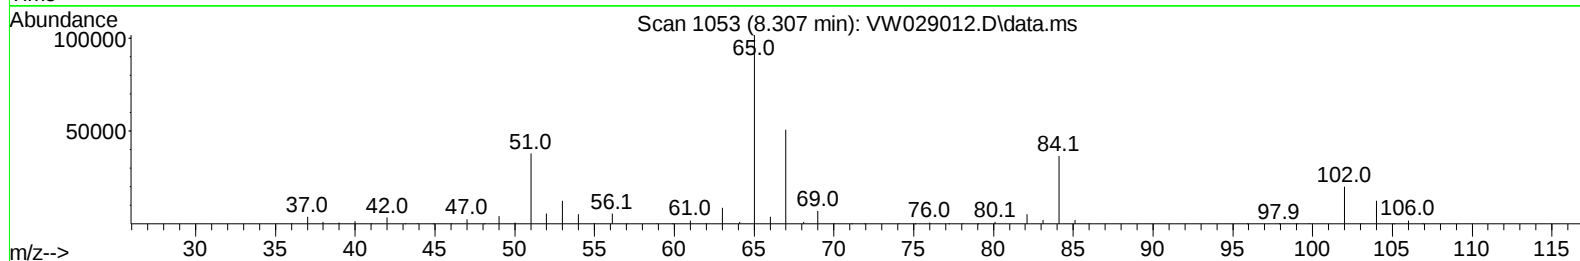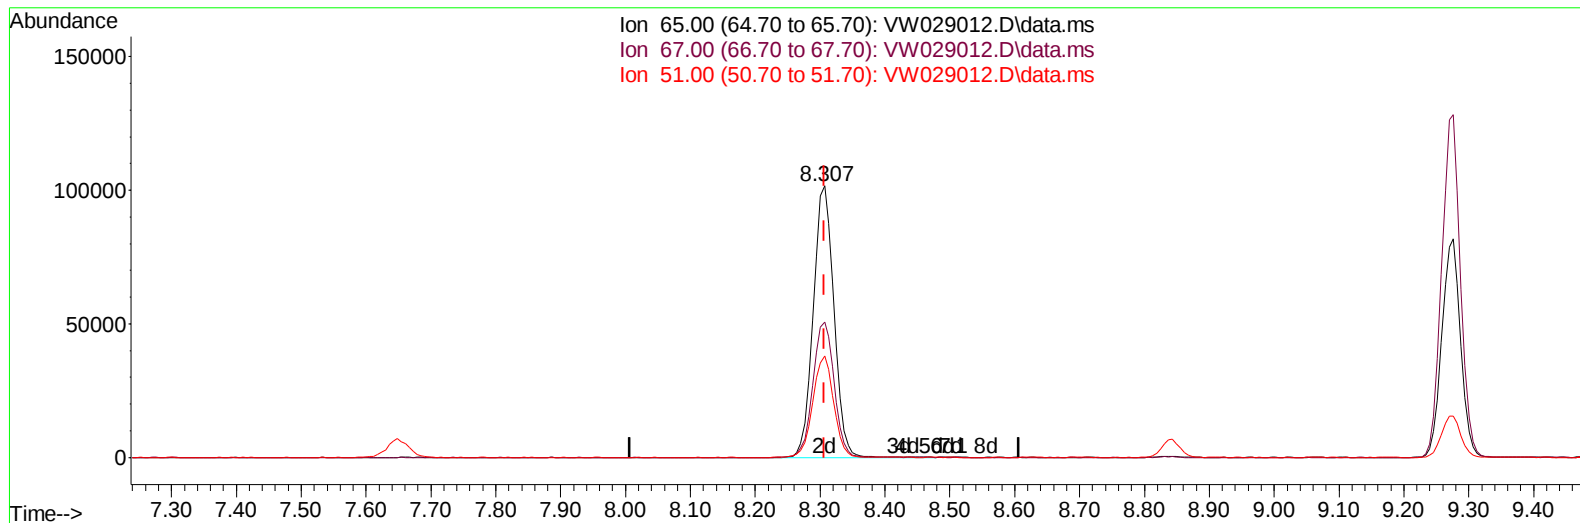

TIC: VW029012.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 24.65 ug/L m

response 224798

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.02#
51.00	105.10	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060524\
 Data File : VW029012.D
 Acq On : 05 Jun 2024 11:09
 Operator : SY/MD
 Sample : P2710-10
 Misc : 5.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BL9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/06/2024
 Supervised By :Mahesh Dadoda 06/06/2024

Quant Time: Jun 05 23:50:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 05 23:49:22 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		607248	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		535086	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		217114	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		223622	23.181	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	92.720%	
7) Chloroethane-d5	2.899	69		177439	23.953	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	95.800%	
11) 1,1-Dichloroethene-d2	4.021	65		100170	23.625	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	94.480%	
21) 2-Butanone-d5	7.075	46		96595	49.008	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	98.020%	
24) Chloroform-d	7.648	84		406327	23.454	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4	8.307	65		224798m	24.647	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	98.600%	
32) Benzene-d6	8.276	84		844608	25.717	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	102.880%	
36) 1,2-Dichloropropane-d6	9.276	67		257622	25.872	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	103.480%	
41) Toluene-d8	10.325	98		759710	25.922	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	103.680%	
43) trans-1,3-Dichloroprop...	10.575	79		93868	24.532	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	98.120%	
47) 2-Hexanone-d5	10.922	63		69914	53.205	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	106.400%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		167912	24.273	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	97.080%	
66) 1,2-Dichlorobenzene-d4	13.848	152		201914	26.207	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	104.840%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060524\
Data File : VW029012.D
Acq On : 05 Jun 2024 11:09
Operator : SY/MD
Sample : P2710-10
Misc : 5.03g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BL9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/06/2024
Supervised By :Mahesh Dadoda 06/06/2024

Quant Time: Jun 05 23:50:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 05 23:49:22 2024
Response via : Initial Calibration

