

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060622\
 Data File : VW023402.D
 Acq On : 06 Jun 2022 15:17
 Operator : SY/VA
 Sample : VW0606SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK523

Quant Time: Jun 07 01:57:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 07 01:56:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	382103	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	347379	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	163436	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	160177	27.082	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.320%
7) Chloroethane-d5	2.885	69	113804	27.314	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.240%
11) 1,1-Dichloroethene-d2	4.019	63	167066	18.809	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.240%
21) 2-Butanone-d5	7.080	46	56451	49.489	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.980%
24) Chloroform-d	7.653	84	246354	23.910	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.640%
26) 1,2-Dichloroethane-d4	8.305	65	138738	25.633	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.520%
32) Benzene-d6	8.274	84	495551	25.698	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.800%
36) 1,2-Dichloropropane-d6	9.274	67	140807	26.052	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.200%
41) Toluene-d8	10.323	98	473572	25.787	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.160%
43) trans-1,3-Dichloroprop...	10.579	79	58832	24.398	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.600%
47) 2-Hexanone-d5	10.926	63	43400	53.645	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.280%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	113773	24.602	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	13.853	152	147117	24.869	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.480%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.042	75	5461	0.730	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060622\
Data File : VW023402.D
Acq On : 06 Jun 2022 15:17
Operator : SY/VA
Sample : VW0606SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK523

Quant Time: Jun 07 01:57:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 07 01:56:30 2022
Response via : Initial Calibration

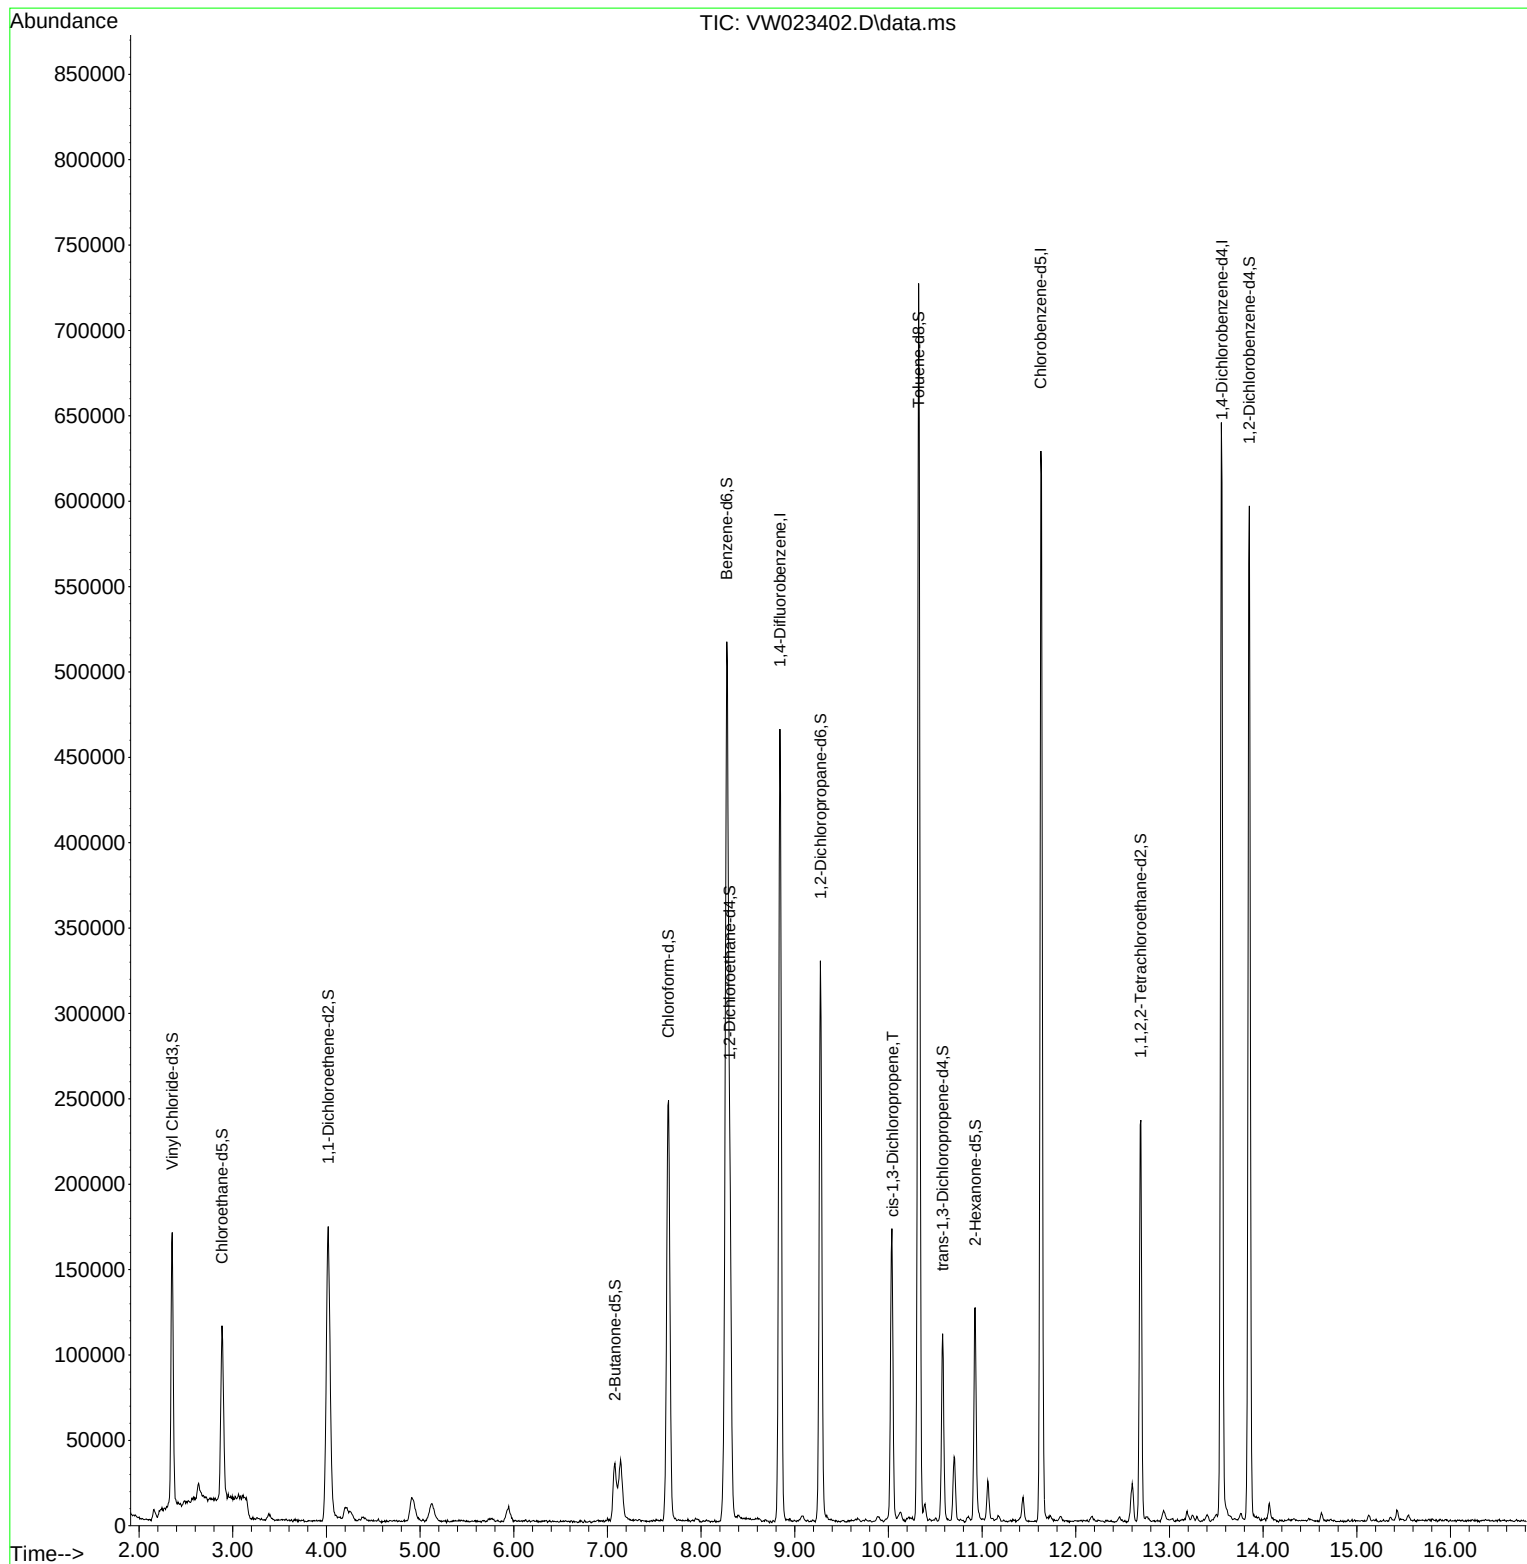

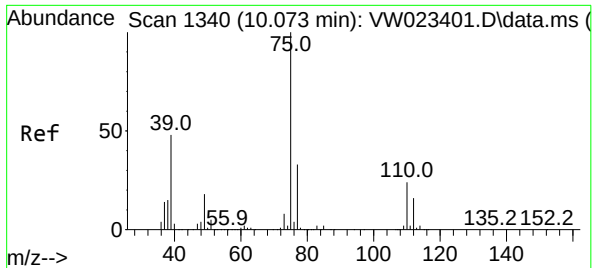

#39
 cis-1,3-Dichloropropene
 Concen: 0.730 ug/L
 RT: 10.042 min Scan# 11
 Delta R.T. -0.031 min
 Lab File: VW023402.D
 Acq: 06 Jun 2022 15:17

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK523

Tgt Ion: 75 Resp: 5461
 Ion Ratio Lower Upper
 75 100
 77 37.3 22.1 41.1

