

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060622\
 Data File : VW023403.D
 Acq On : 06 Jun 2022 15:41
 Operator : SY/VA
 Sample : N3171-13
 Misc : 5.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Jun 07 01:57:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 07 01:56:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	367543	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	338544	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	155583	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	153166	26.922	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.680%
7) Chloroethane-d5	2.885	69	108856	27.161	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.640%
11) 1,1-Dichloroethene-d2	4.019	63	159731	18.696	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.800%
21) 2-Butanone-d5	7.074	46	61348	55.912	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.820%
24) Chloroform-d	7.653	84	239342	24.150	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.600%
26) 1,2-Dichloroethane-d4	8.305	65	135972	26.117	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.480%
32) Benzene-d6	8.275	84	483604	25.733	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.920%
36) 1,2-Dichloropropane-d6	9.274	67	137201	26.048	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.200%
41) Toluene-d8	10.323	98	457496	25.561	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.240%
43) trans-1,3-Dichloroprop...	10.579	79	57756	24.577	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.320%
47) 2-Hexanone-d5	10.920	63	47692	60.488	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.980%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	118253	26.239	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	139477	24.768	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.080%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4912	0.673	ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060622\
Data File : VW023403.D
Acq On : 06 Jun 2022 15:41
Operator : SY/VA
Sample : N3171-13
Misc : 5.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Jun 07 01:57:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060622SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 07 01:56:30 2022
Response via : Initial Calibration

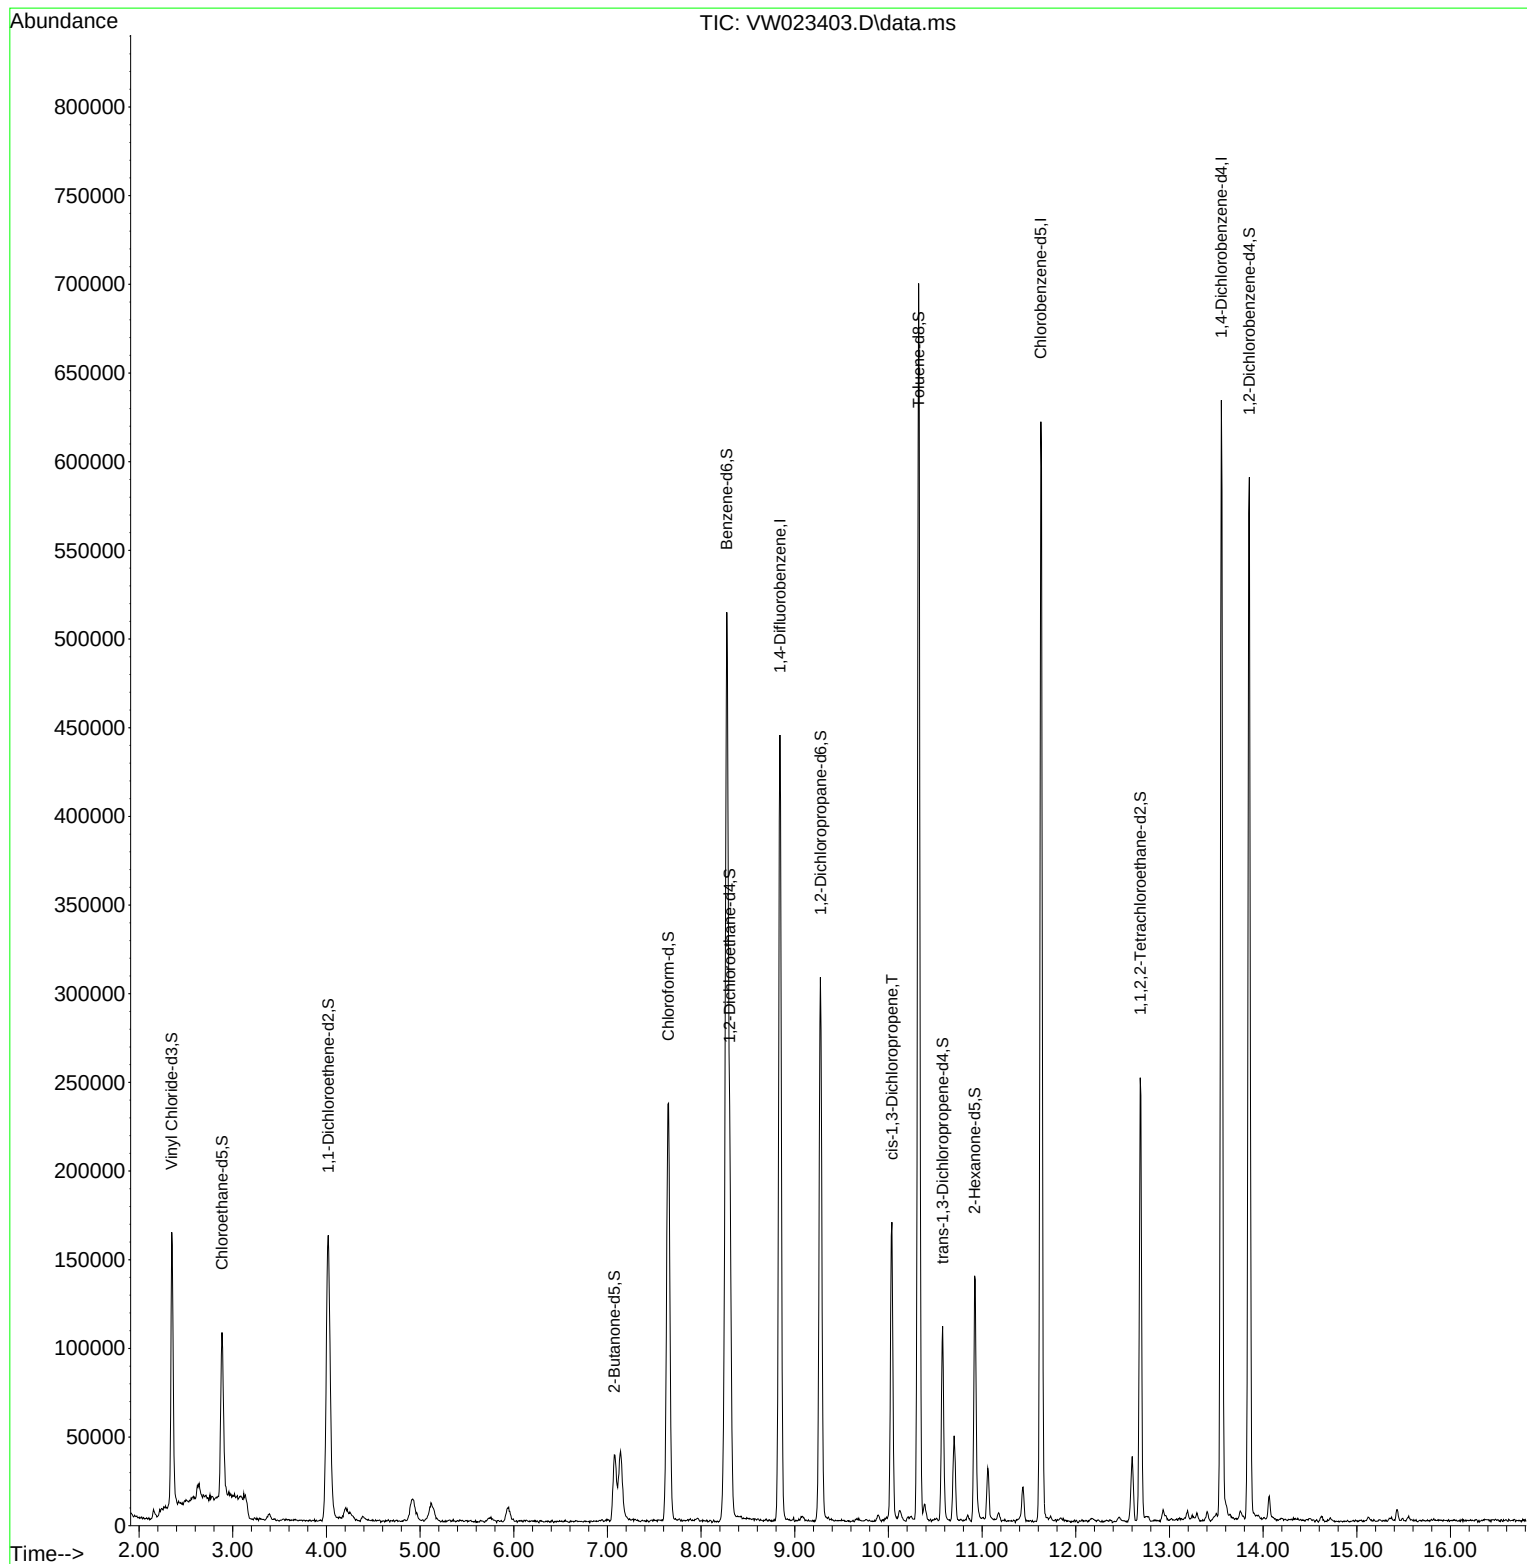

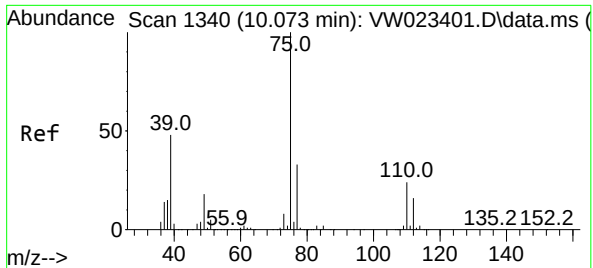

#39
 cis-1,3-Dichloropropene
 Concen: 0.673 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023403.D
 Acq: 06 Jun 2022 15:41

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Tgt Ion: 75 Resp: 4912
 Ion Ratio Lower Upper
 75 100
 77 50.5 22.1 41.1#

