

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026108.D
 Acq On : 06 Jun 2023 15:36
 Operator : SY/MD
 Sample : 03062-01
 Misc : 4.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EZEK9

Manual IntegrationsAPPROVED

Quant Time: Jun 07 01:07:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

06/07/2023
 Supervised By :Mahesh
 Dadoda

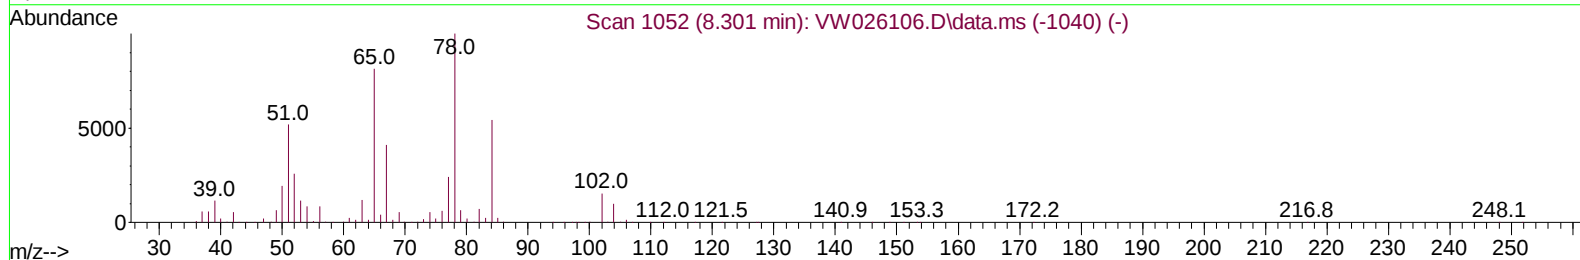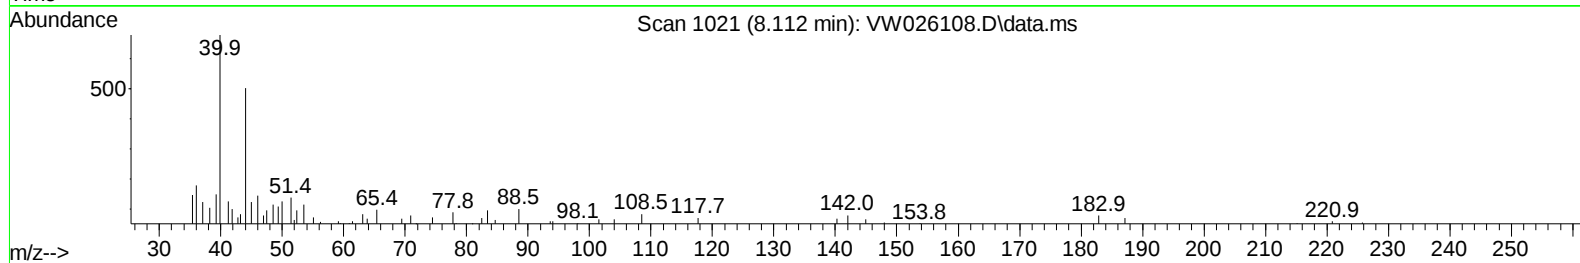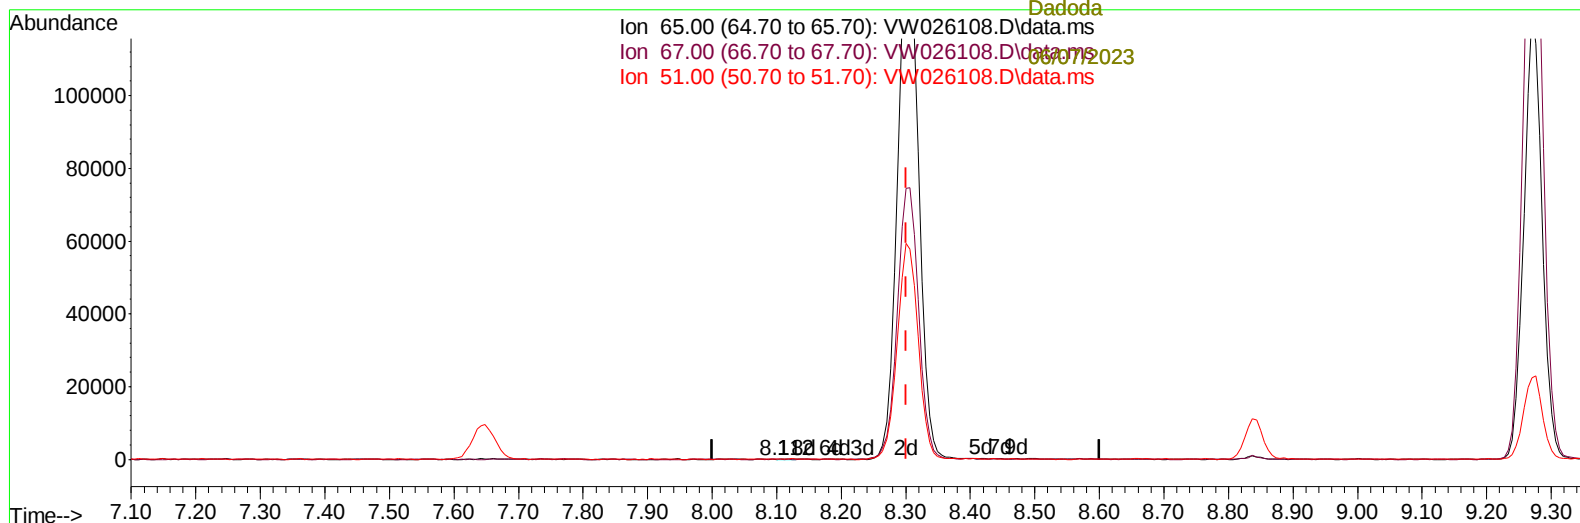

TIC: VW026108.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.112min (-0.189) 0.01 ug/L

response 148

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	37.16
51.00	106.50	92.57
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026108.D
 Acq On : 06 Jun 2023 15:36
 Operator : SY/MD
 Sample : 03062-01
 Misc : 4.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EZEK9

Manual IntegrationsAPPROVED

Quant Time: Jun 07 01:07:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

06/07/2023
 Supervised By :Mahesh
 Dadoda

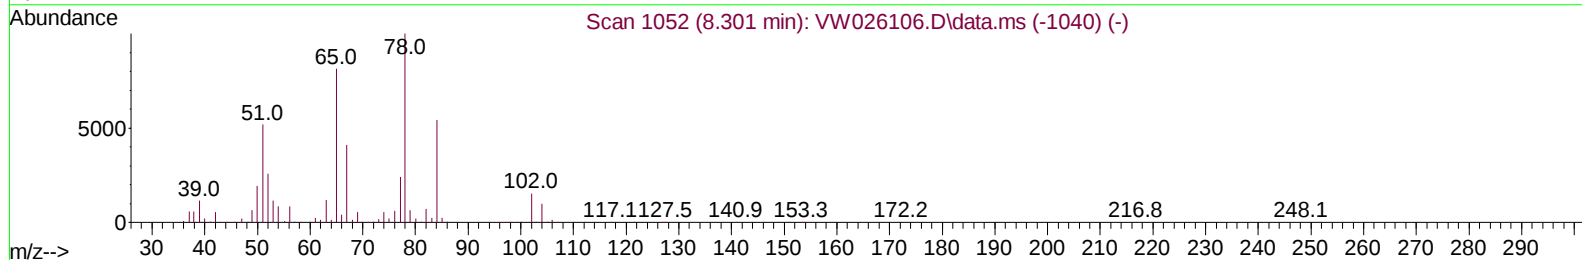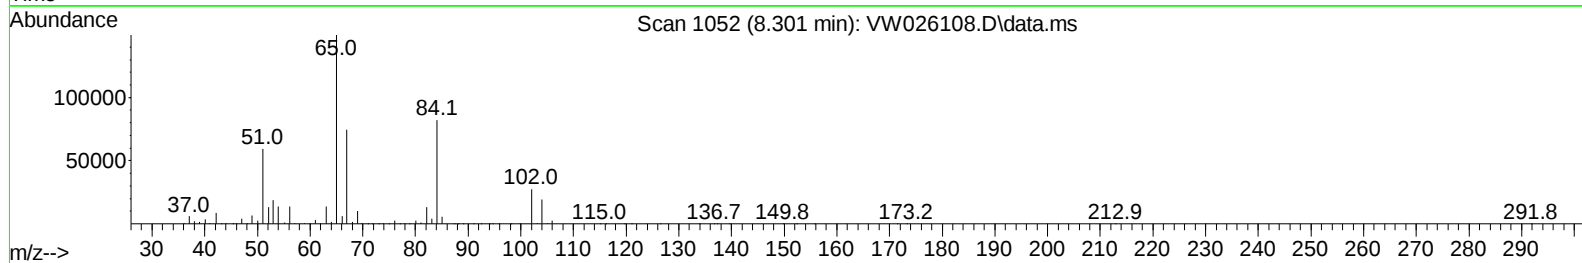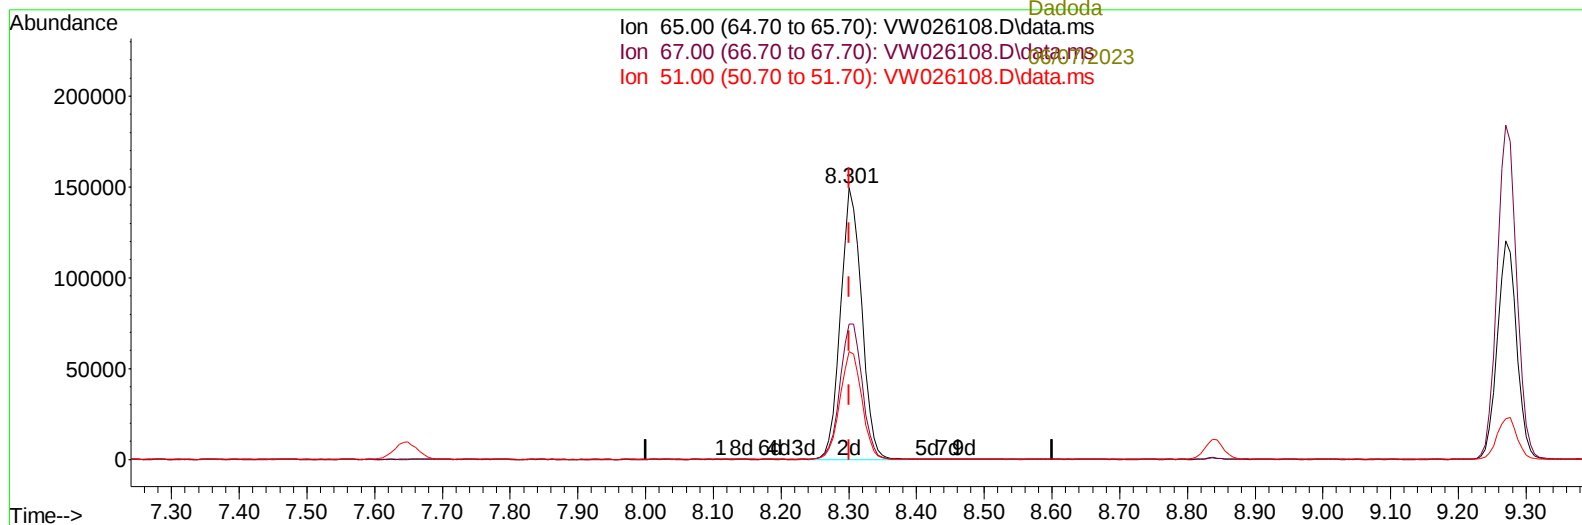

TIC: VW026108.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.301min (+ 0.000) 21.38 ug/L m

response 323884

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	0.02#
51.00	106.50	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026108.D
 Acq On : 06 Jun 2023 15:36
 Operator : SY/MD
 Sample : 03062-01
 Misc : 4.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEK9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

06/07/2023
 Supervised By :Mahesh
 Dadoda

Quant Time: Jun 07 01:07:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----06/07/2023						
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	945897	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	833178	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	381335	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	281651	21.166	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.680%	
7) Chloroethane-d5	2.899	69	230679	23.158	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	92.640%	
11) 1,1-Dichloroethene-d2	4.021	65	131656	20.065	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	80.280%	
21) 2-Butanone-d5	7.075	46	187976	48.522	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	97.040%	
24) Chloroform-d	7.642	84	558169	20.151	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	80.600%	
26) 1,2-Dichloroethane-d4	8.301	65	323884m	21.384	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	85.520%	
32) Benzene-d6	8.270	84	1120709	19.990	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	79.960%	
36) 1,2-Dichloropropane-d6	9.270	67	370432	20.856	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	83.440%	
41) Toluene-d8	10.319	98	970692	19.524	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	78.080%	
43) trans-1,3-Dichloroprop...	10.575	79	136785	19.434	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.720%	
47) 2-Hexanone-d5	10.922	63	125209	44.708	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.420%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	293872	22.737	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	90.960%	
66) 1,2-Dichlorobenzene-d4	13.849	152	305827	20.953	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	83.800%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
Data File : VW026108.D
Acq On : 06 Jun 2023 15:36
Operator : SY/MD
Sample : 03062-01
Misc : 4.58g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZEK9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

06/07/2023
Supervised By :Mahesh
Dadoda

06/07/2023

