




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026112.D
 Acq On : 06 Jun 2023 17:13
 Operator : SY/MD
 Sample : 03062-08
 Misc : 4.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL4

Manual IntegrationsAPPROVED

Quant Time: Jun 07 01:08:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2023
 Supervised By :Mahesh Dadoda 06/07/2023

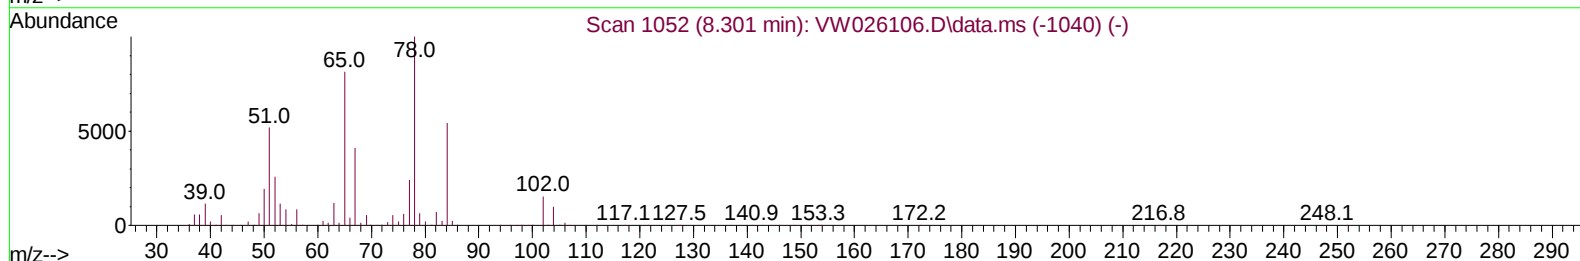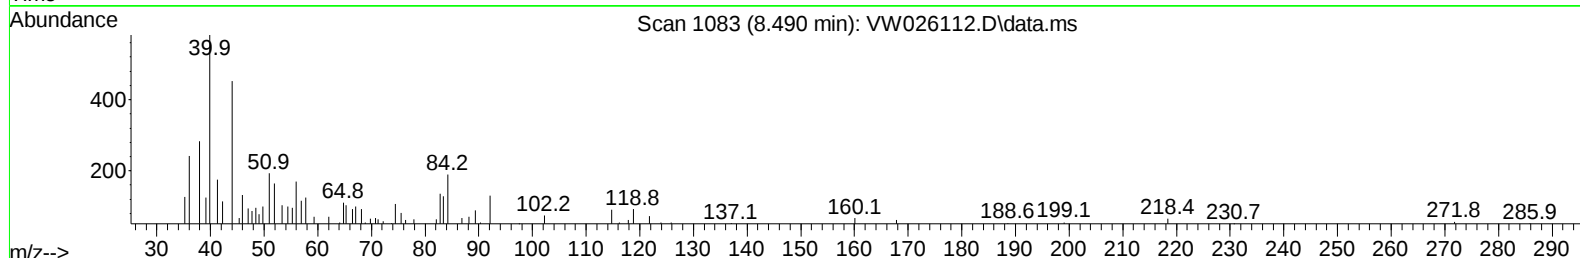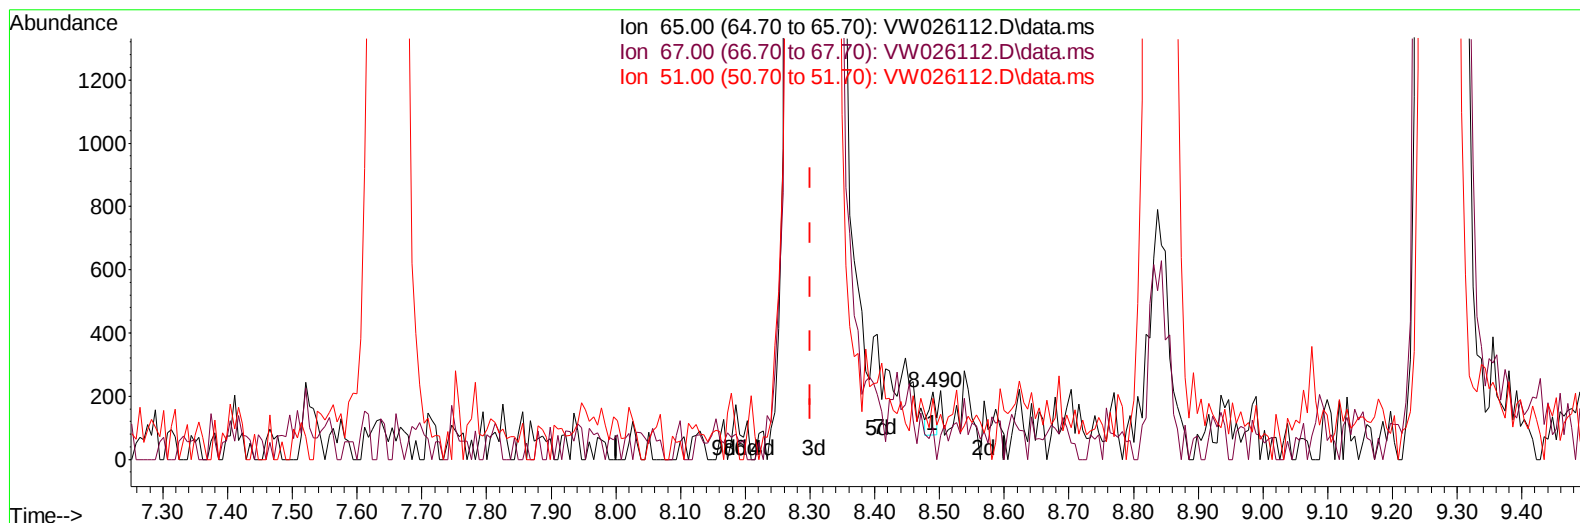

TIC: VW026112.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.490min (+ 0.189) 0.01 ug/L

response 99

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	37.37
51.00	106.50	89.90
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026112.D
 Acq On : 06 Jun 2023 17:13
 Operator : SY/MD
 Sample : 03062-08
 Misc : 4.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL4

Manual IntegrationsAPPROVED

Quant Time: Jun 07 01:08:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2023
 Supervised By :Mahesh Dadoda 06/07/2023

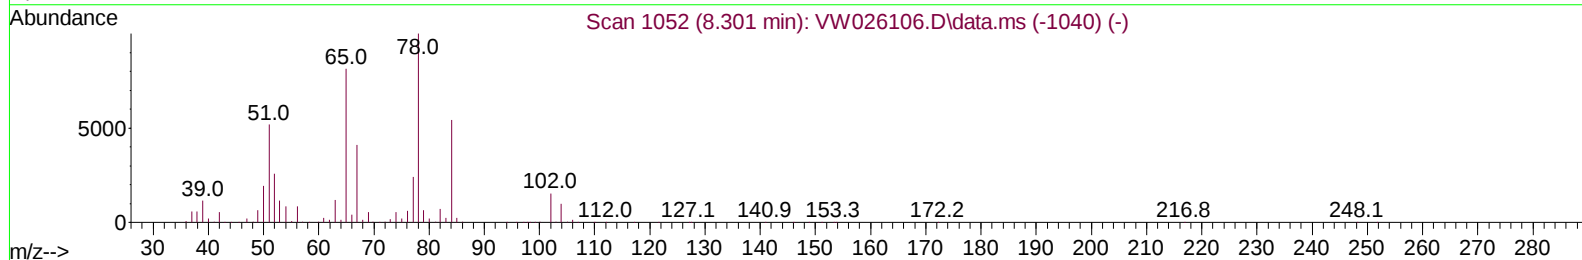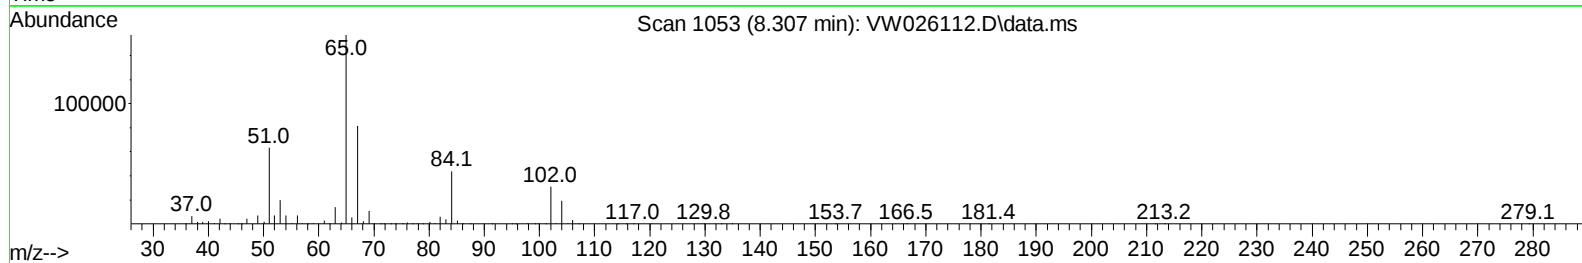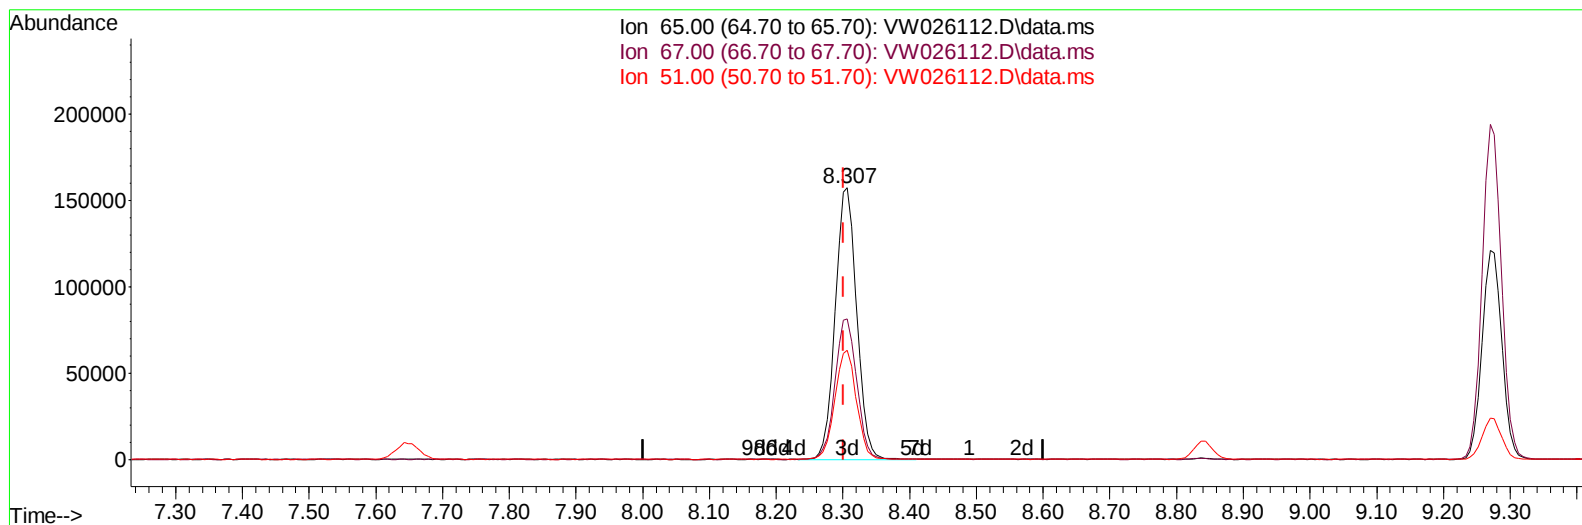

TIC: VW026112.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 23.35 ug/L m

response 350290

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	0.01#
51.00	106.50	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026112.D
 Acq On : 06 Jun 2023 17:13
 Operator : SY/MD
 Sample : 03062-08
 Misc : 4.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL4

Manual IntegrationsAPPROVED

Quant Time: Jun 07 01:08:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2023
 Supervised By :Mahesh Dadoda 06/07/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		937059	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		840643	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		363938	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		267683	20.306	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.240%		
7) Chloroethane-d5	2.893	69		224429	22.743	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	90.960%		
11) 1,1-Dichloroethene-d2	4.021	65		130267	20.041	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	80.160%		
21) 2-Butanone-d5	7.075	46		223627	58.268	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	116.540%		
24) Chloroform-d	7.648	84		578718	21.090	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	84.360%		
26) 1,2-Dichloroethane-d4	8.307	65		350290m	23.345	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	93.400%		
32) Benzene-d6	8.276	84		1172999	20.737	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	82.960%		
36) 1,2-Dichloropropane-d6	9.270	67		392487	21.902	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	87.600%		
41) Toluene-d8	10.325	98		1003730	20.009	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	80.040%		
43) trans-1,3-Dichloroprop...	10.575	79		146273	20.598	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	82.400%		
47) 2-Hexanone-d5	10.922	63		153189	54.213	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	108.420%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		334372	25.641	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	102.560%		
66) 1,2-Dichlorobenzene-d4	13.848	152		315508	22.650	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	90.600%		
Target Compounds							
13) Acetone	4.125	43		8288	2.791	ug/L	Qvalue 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
Data File : VW026112.D
Acq On : 06 Jun 2023 17:13
Operator : SY/MD
Sample : 03062-08
Misc : 4.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZEL4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2023
Supervised By :Mahesh Dadoda 06/07/2023

Quant Time: Jun 07 01:08:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 07 01:06:46 2023
Response via : Initial Calibration

