




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026115.D
 Acq On : 06 Jun 2023 18:25
 Operator : SY/MD
 Sample : 03062-03
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL1

Manual IntegrationsAPPROVED

Quant Time: Jun 07 01:09:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2023
 Supervised By :Mahesh Dadoda 06/07/2023

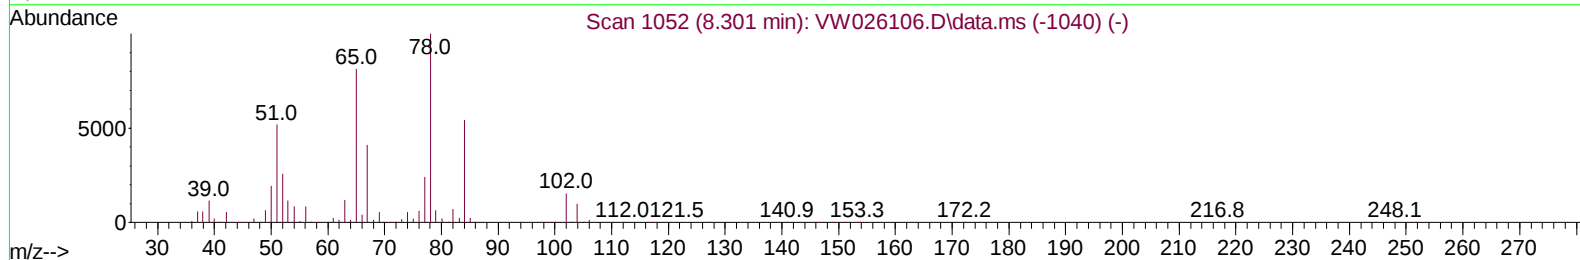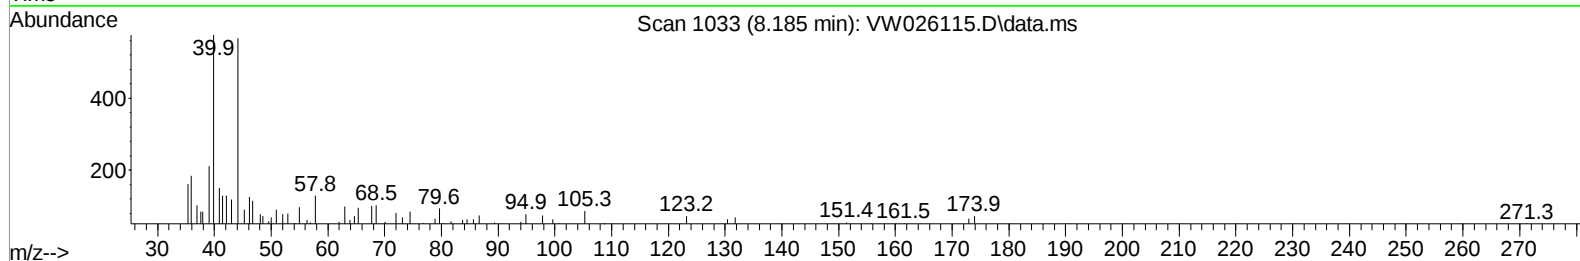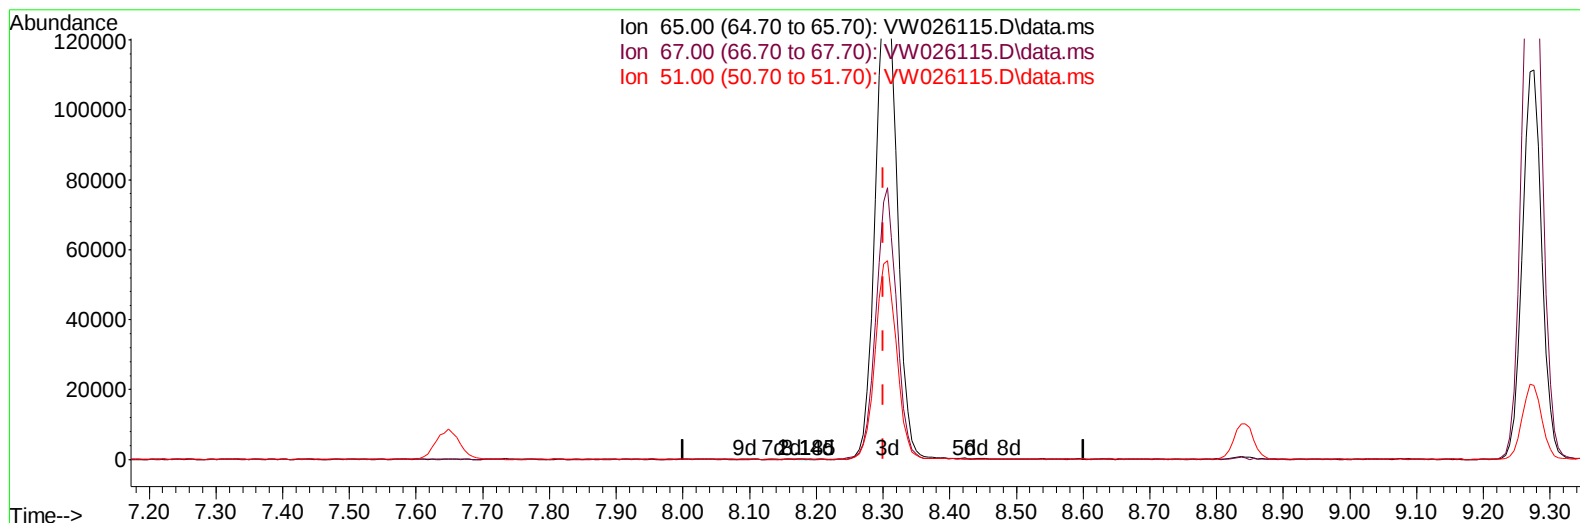

TIC: VW026115.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.185min (-0.116) 0.01 ug/L

response 91

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	50.55
51.00	106.50	98.90
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026115.D
 Acq On : 06 Jun 2023 18:25
 Operator : SY/MD
 Sample : 03062-03
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2023
 Supervised By :Mahesh Dadoda 06/07/2023

Quant Time: Jun 07 01:09:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

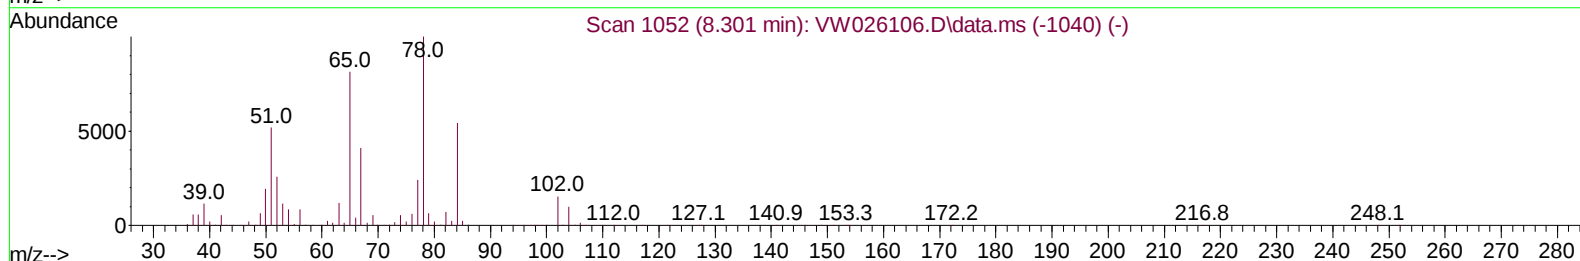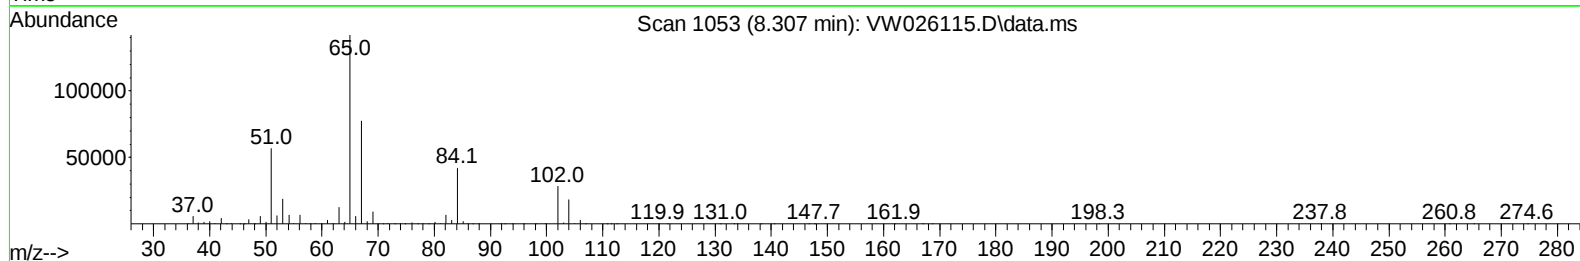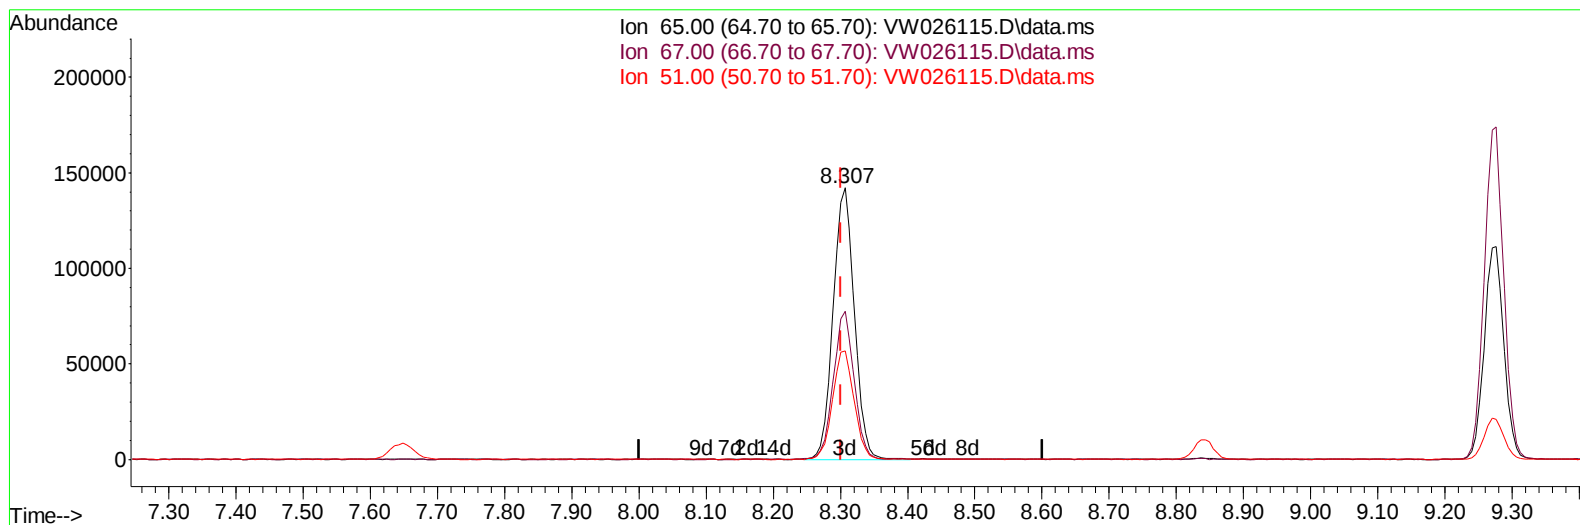

TIC: VW026115.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 21.57 ug/L m

response 311198

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	0.01#
51.00	106.50	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026115.D
 Acq On : 06 Jun 2023 18:25
 Operator : SY/MD
 Sample : 03062-03
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL1

Manual IntegrationsAPPROVED

Quant Time: Jun 07 01:09:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2023
 Supervised By :Mahesh Dadoda 06/07/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		900976	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		820418	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		360855	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		240322	18.961	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	75.840%	
7) Chloroethane-d5	2.899	69		203562	21.454	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	85.800%	
11) 1,1-Dichloroethene-d2	4.021	65		118455	18.953	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	75.800%	
21) 2-Butanone-d5	7.075	46		196763	53.322	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	106.640%	
24) Chloroform-d	7.648	84		516444	19.574	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	78.280%	
26) 1,2-Dichloroethane-d4	8.307	65		311198m	21.570	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	86.280%	
32) Benzene-d6	8.276	84		1038212	18.807	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	75.240%	
36) 1,2-Dichloropropane-d6	9.276	67		350679	20.051	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	80.200%	
41) Toluene-d8	10.325	98		892013	18.220	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	72.880%	
43) trans-1,3-Dichloroprop...	10.575	79		127623	18.415	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	73.640%	
47) 2-Hexanone-d5	10.922	63		133496	48.408	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	96.820%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		289900	22.779	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	91.120%	
66) 1,2-Dichlorobenzene-d4	13.848	152		284322	20.585	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	82.360%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
Data File : VW026115.D
Acq On : 06 Jun 2023 18:25
Operator : SY/MD
Sample : 03062-03
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZEL1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2023
Supervised By :Mahesh Dadoda 06/07/2023

Quant Time: Jun 07 01:09:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 07 01:06:46 2023
Response via : Initial Calibration

