

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
 Data File : VW026112.D
 Acq On : 06 Jun 2023 17:13
 Operator : SY/MD
 Sample : 03062-08
 Misc : 4.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2023
 Supervised By :Mahesh Dadoda 06/07/2023

Quant Time: Jun 07 01:08:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 07 01:06:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	937059	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	840643	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	363938	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	267683	20.306	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.240%		
7) Chloroethane-d5	2.893	69	224429	22.743	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.960%		
11) 1,1-Dichloroethene-d2	4.021	65	130267	20.041	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	80.160%		
21) 2-Butanone-d5	7.075	46	223627	58.268	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	116.540%		
24) Chloroform-d	7.648	84	578718	21.090	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.360%		
26) 1,2-Dichloroethane-d4	8.307	65	350290m	23.345	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	93.400%		
32) Benzene-d6	8.276	84	1172999	20.737	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	82.960%		
36) 1,2-Dichloropropane-d6	9.270	67	392487	21.902	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	87.600%		
41) Toluene-d8	10.325	98	1003730	20.009	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.040%		
43) trans-1,3-Dichloroprop...	10.575	79	146273	20.598	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.400%		
47) 2-Hexanone-d5	10.922	63	153189	54.213	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	108.420%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	334372	25.641	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	102.560%		
66) 1,2-Dichlorobenzene-d4	13.848	152	315508	22.650	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.600%		
Target Compounds					Qvalue	
13) Acetone	4.125	43	8288	2.791	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060623\
Data File : VW026112.D
Acq On : 06 Jun 2023 17:13
Operator : SY/MD
Sample : 03062-08
Misc : 4.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EZEL4

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2023
Supervised By :Mahesh Dadoda 06/07/2023

Quant Time: Jun 07 01:08:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 07 01:06:46 2023
Response via : Initial Calibration

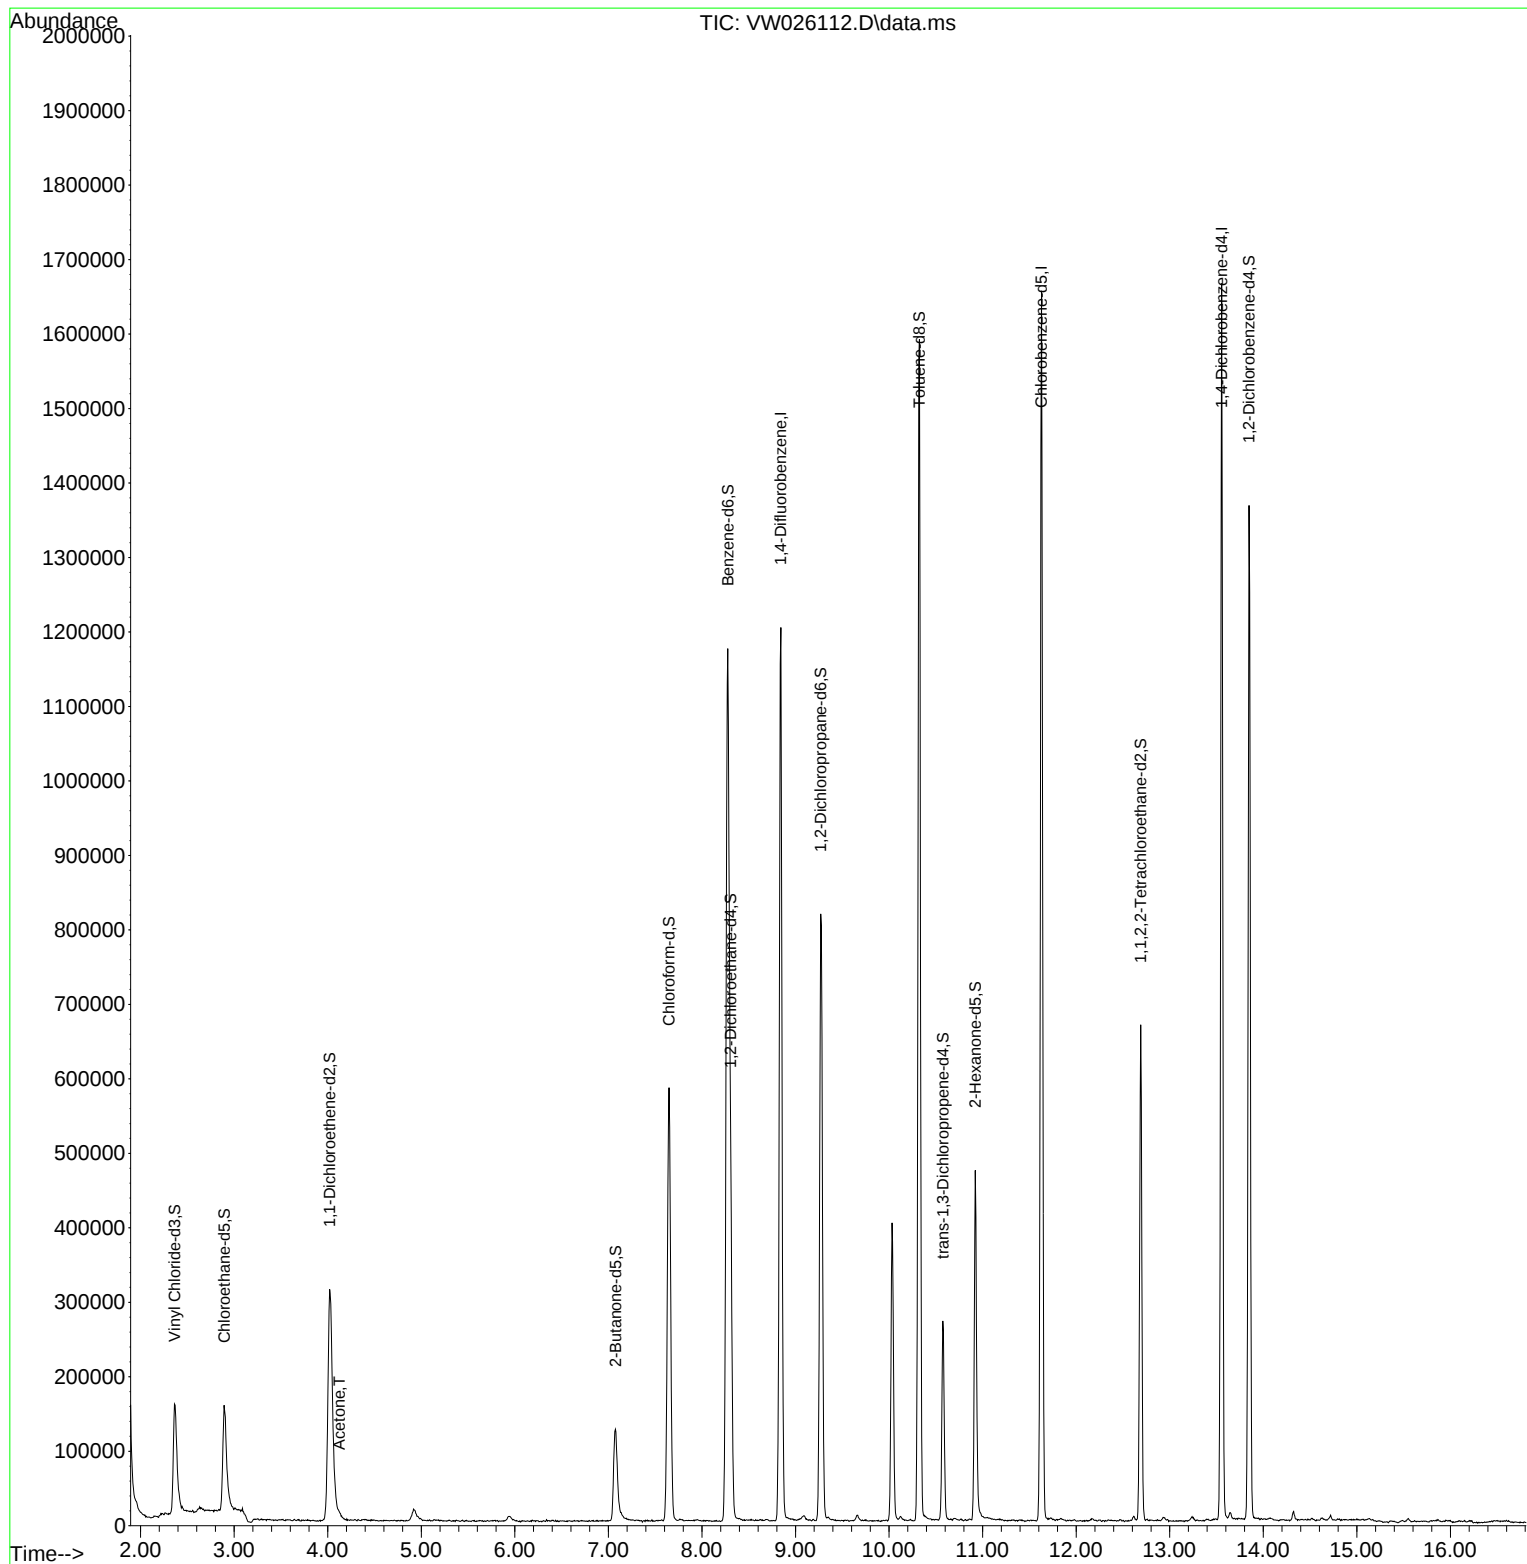

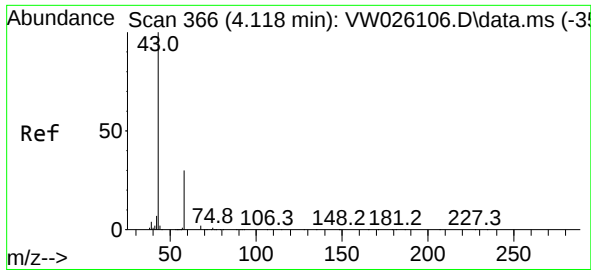

#13
 Acetone
 Concen: 2.791 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW026112.D
 Acq: 06 Jun 2023 17:13

Instrument :
 MSVOA_W
 ClientSampleId :
 EZEL4

Tgt Ion: 43 Resp: 828
 Ion Ratio Lower Upper
 43 100
 58 23.1 0.0 58.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2023
 Supervised By :Mahesh Dadoda 06/07/2023

