

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
 Data File : VW029041.D
 Acq On : 06 Jun 2024 16:32
 Operator : SY/MD
 Sample : P2696-12
 Misc : 4.39g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 07 00:26:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 00:21:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	745425	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	655287	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	273682	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	210337	17.762	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.040%
7) Chloroethane-d5	2.899	69	173221	19.049	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.200%
11) 1,1-Dichloroethene-d2	4.021	65	97710	18.773	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.080%
21) 2-Butanone-d5	7.075	46	99624	41.175	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.360%
24) Chloroform-d	7.648	84	431236	20.278	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.120%
26) 1,2-Dichloroethane-d4	8.307	65	233885	20.890	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.560%
32) Benzene-d6	8.276	84	890896	22.151	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.600%
36) 1,2-Dichloropropane-d6	9.270	67	273365	22.417	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.680%
41) Toluene-d8	10.319	98	778139	21.681	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.720%
43) trans-1,3-Dichloroprop...	10.575	79	93470	19.947	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.800%
47) 2-Hexanone-d5	10.922	63	73019	45.375	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.740%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	178046	21.017	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.080%
66) 1,2-Dichlorobenzene-d4	13.848	152	224607	23.127	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.520%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	7013	0.452	ug/L	# 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
Data File : VW029041.D
Acq On : 06 Jun 2024 16:32
Operator : SY/MD
Sample : P2696-12
Misc : 4.39g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 07 00:26:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 07 00:21:46 2024
Response via : Initial Calibration

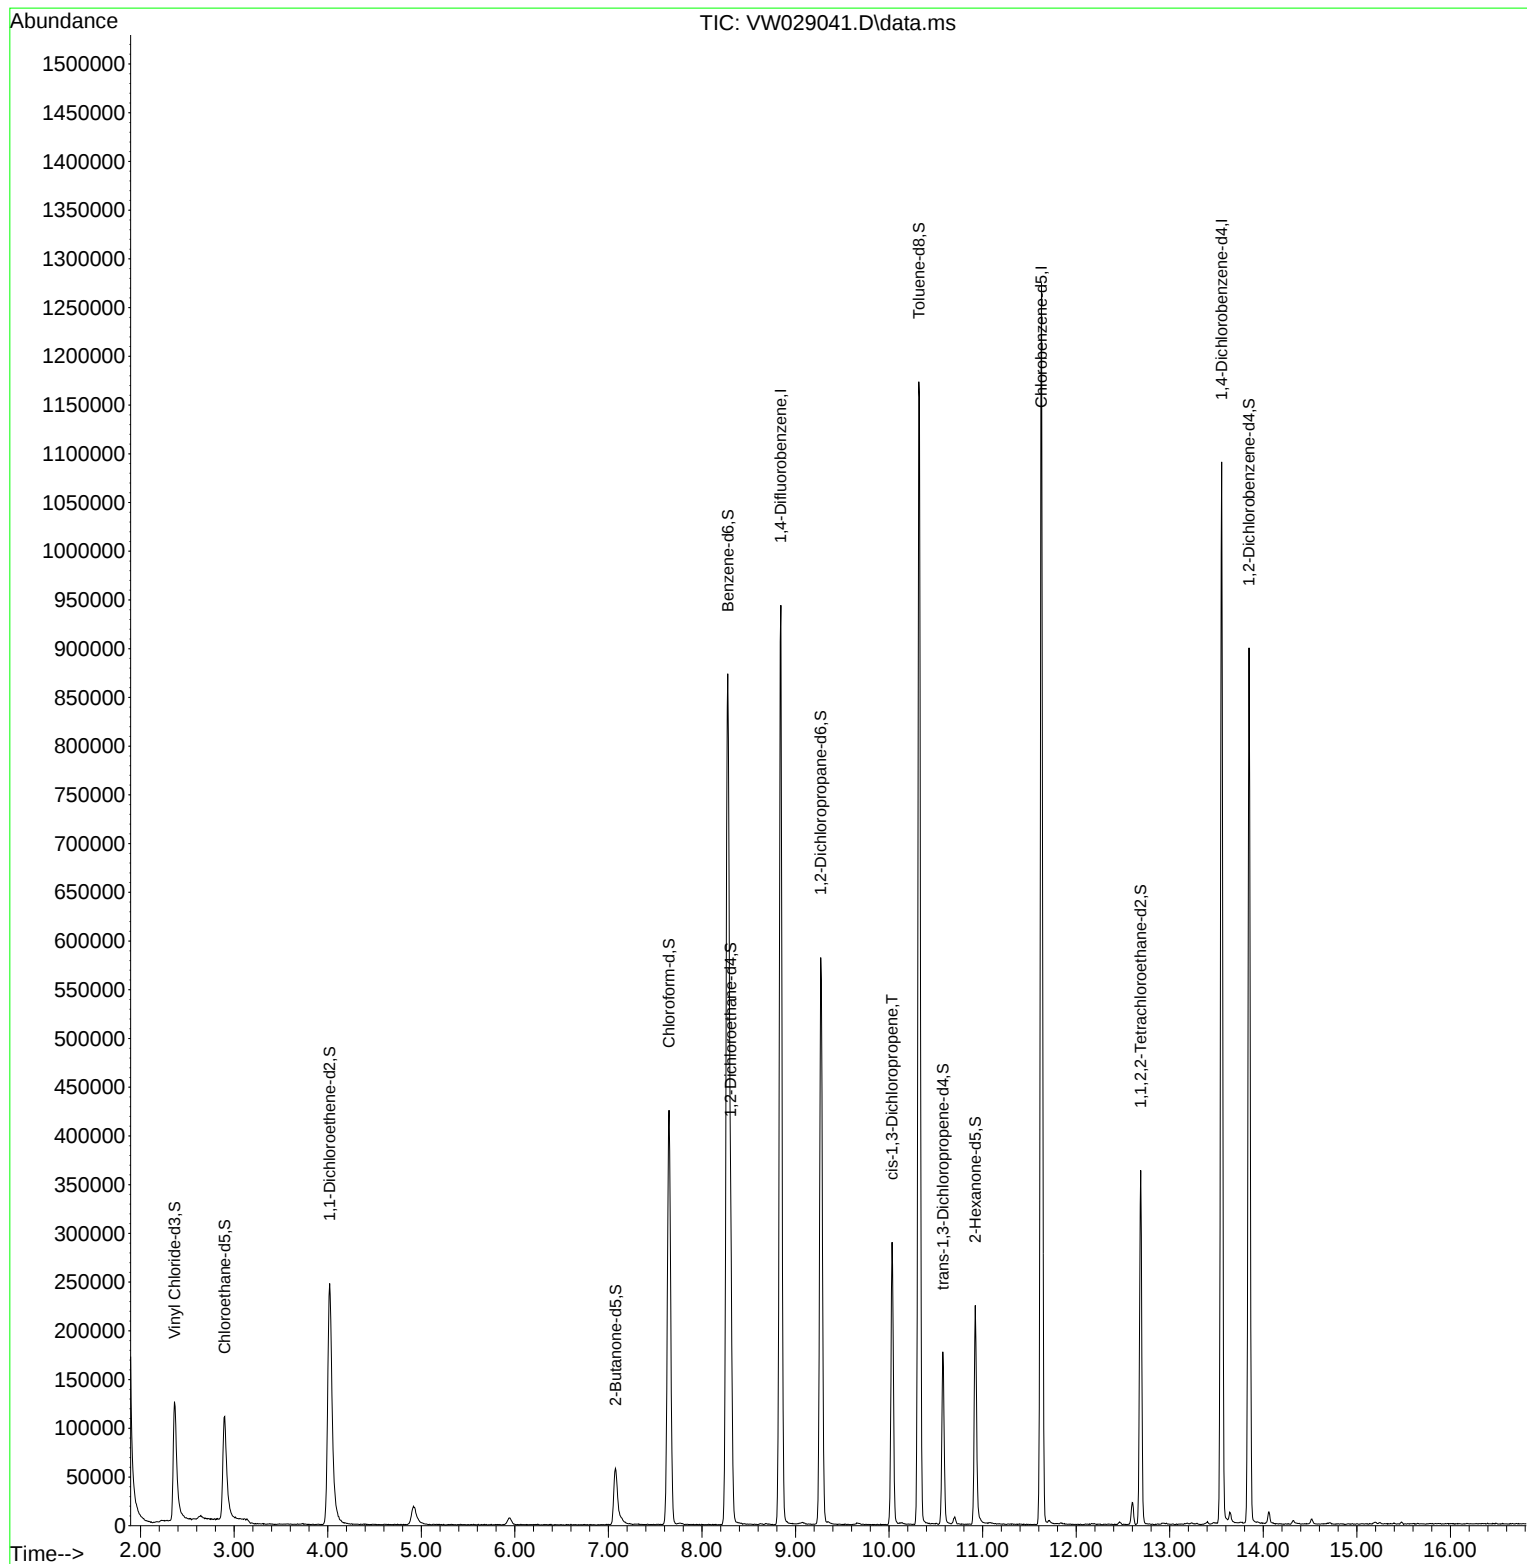

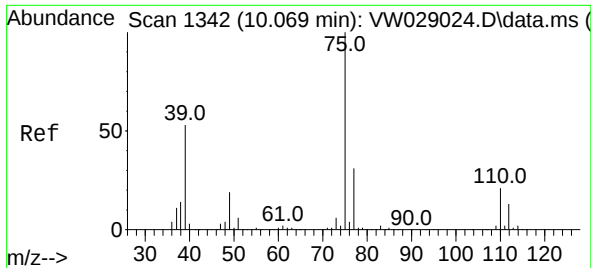

#39
 cis-1,3-Dichloropropene
 Concen: 0.452 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029041.D
 Acq: 06 Jun 2024 16:32

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 7013
 Ion Ratio Lower Upper
 75 100
 77 51.8 21.0 39.0#

