




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
 Data File : VW029035.D
 Acq On : 06 Jun 2024 14:08
 Operator : SY/MD
 Sample : P2710-13RE
 Misc : 4.91g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BM3RE

Manual IntegrationsAPPROVED

Quant Time: Jun 07 00:25:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 00:21:46 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2024
 Supervised By :Mahesh Dadoda 06/07/2024

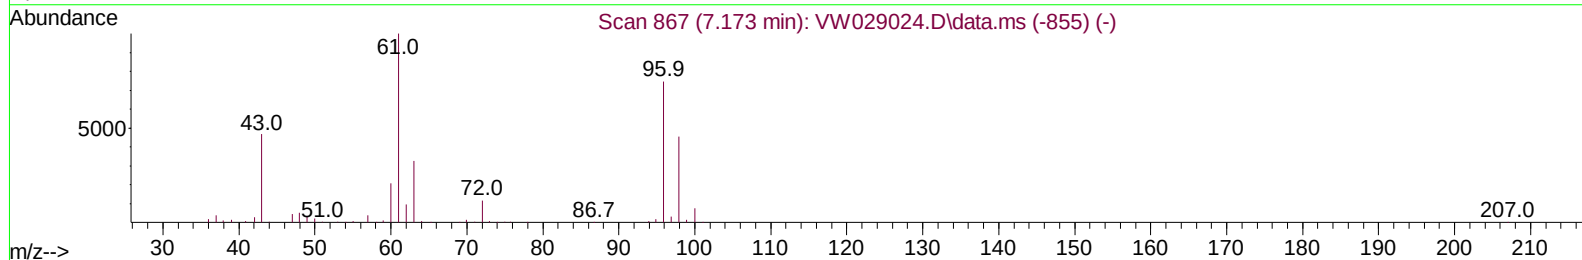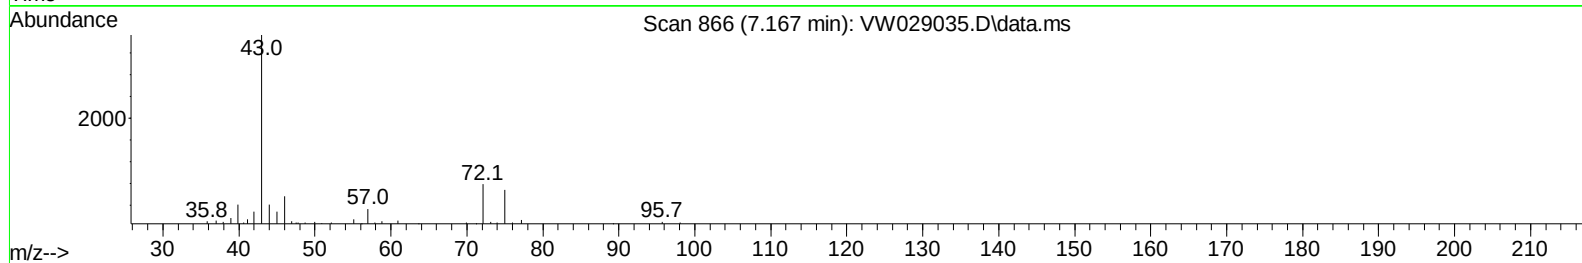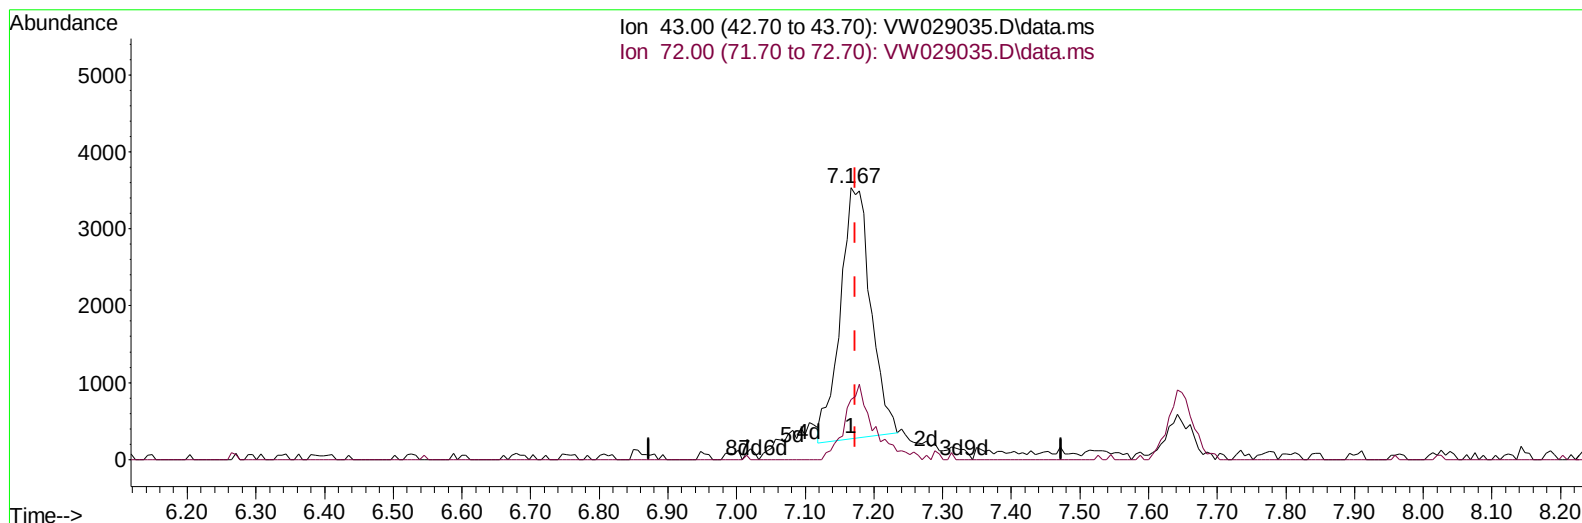

TIC: VW029035.D\data.ms

(22) 2-Butanone (T)

7.167min (-0.006) 5.19 ug/L

response 10095

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	23.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
 Data File : VW029035.D
 Acq On : 06 Jun 2024 14:08
 Operator : SY/MD
 Sample : P2710-13RE
 Misc : 4.91g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BM3RE

Manual IntegrationsAPPROVED

Quant Time: Jun 07 00:25:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 00:21:46 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2024
 Supervised By :Mahesh Dadoda 06/07/2024

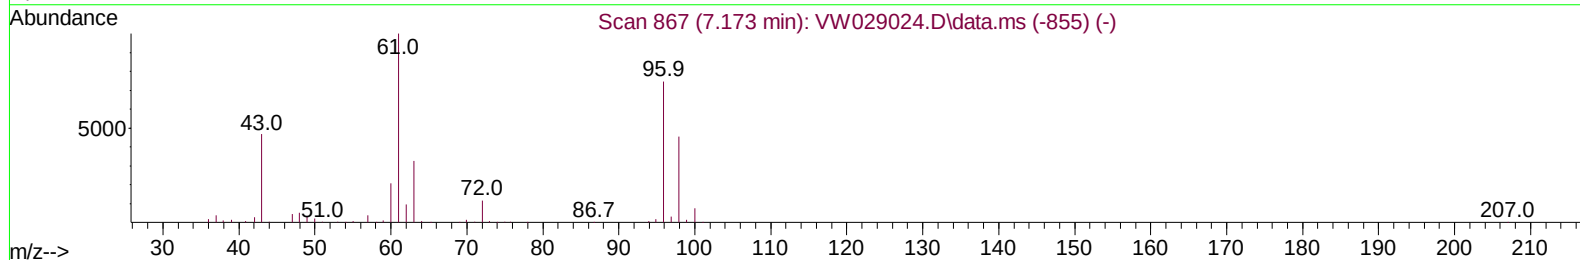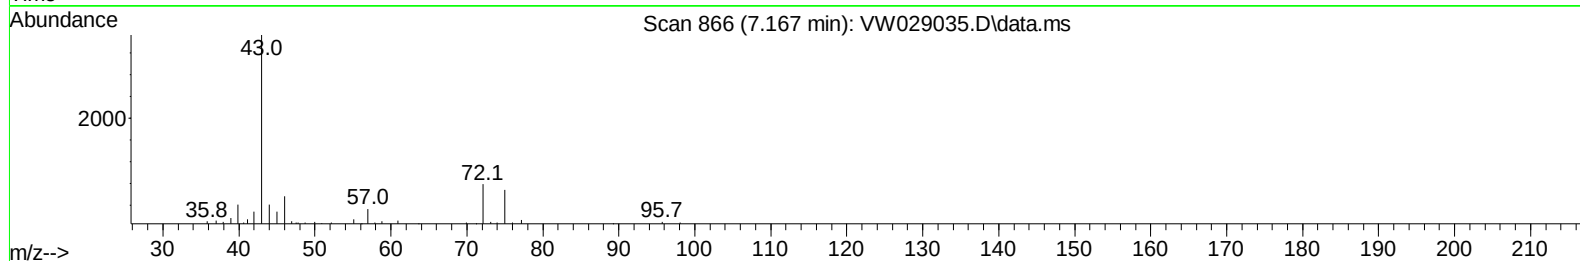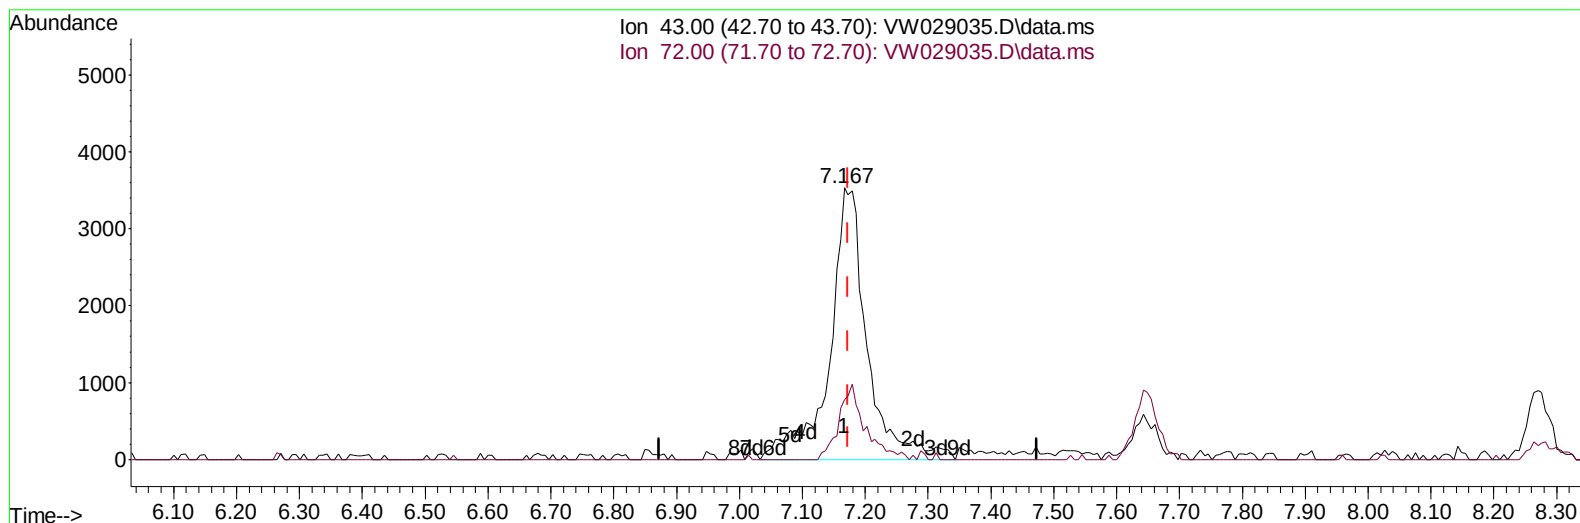

TIC: VW029035.D\data.ms

(22) 2-Butanone (T)

7.167min (-0.006) 7.57 ug/L m

response 14738

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	16.35
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
 Data File : VW029035.D
 Acq On : 06 Jun 2024 14:08
 Operator : SY/MD
 Sample : P2710-13RE
 Misc : 4.91g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BM3RE

Manual IntegrationsAPPROVED

Quant Time: Jun 07 00:25:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 00:21:46 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2024
 Supervised By :Mahesh Dadoda 06/07/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		474936	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		314590	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		71104	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		184155	24.408	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	97.640%		
7) Chloroethane-d5	2.899	69		149042	25.724	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	102.880%		
11) 1,1-Dichloroethene-d2	4.021	65		76858	23.176	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	92.720%		
21) 2-Butanone-d5	7.069	46		93632	60.739	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	121.480%		
24) Chloroform-d	7.648	84		327554	24.175	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	96.680%		
26) 1,2-Dichloroethane-d4	8.301	65		188824	26.471	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	105.880%		
32) Benzene-d6	8.270	84		660178	34.191	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	136.760%#		
36) 1,2-Dichloropropane-d6	9.270	67		201067	34.345	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	137.360%#		
41) Toluene-d8	10.319	98		491670	28.535	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	114.120%		
43) trans-1,3-Dichloroprop...	10.575	79		63779	28.352	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	113.400%		
47) 2-Hexanone-d5	10.922	63		62182	80.488	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	160.980%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		106242	26.123	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	104.480%		
66) 1,2-Dichlorobenzene-d4	13.849	152		58713	23.269	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	93.080%		
Target Compounds							
13) Acetone	4.119	43		26861	16.627	ug/L	99
22) 2-Butanone	7.167	43		14738m	7.571	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
Data File : VW029035.D
Acq On : 06 Jun 2024 14:08
Operator : SY/MD
Sample : P2710-13RE
Misc : 4.91g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BM3RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2024
Supervised By :Mahesh Dadoda 06/07/2024

Quant Time: Jun 07 00:25:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 07 00:21:46 2024
Response via : Initial Calibration

