




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
 Data File : VW029044.D
 Acq On : 06 Jun 2024 17:44
 Operator : SY/MD
 Sample : P2696-08RE
 Misc : 4.43g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BN7RE

Manual IntegrationsAPPROVED

Quant Time: Jun 07 00:27:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 00:21:46 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2024
 Supervised By :Mahesh Dadoda 06/07/2024

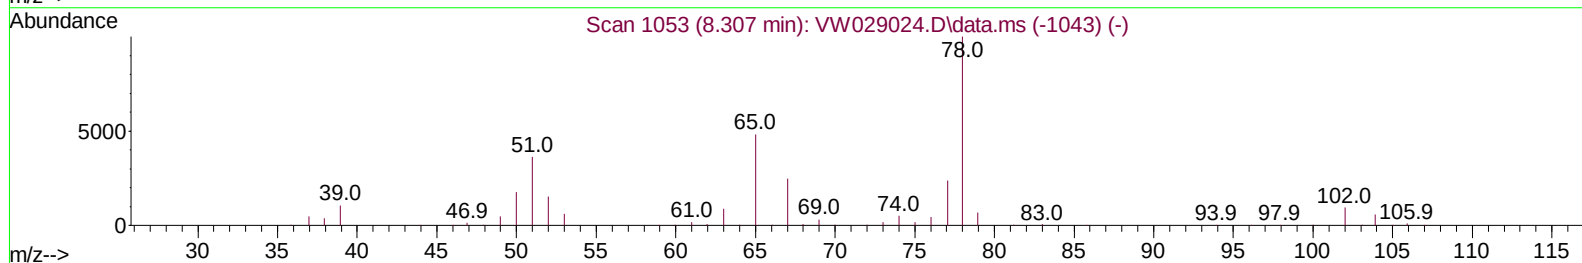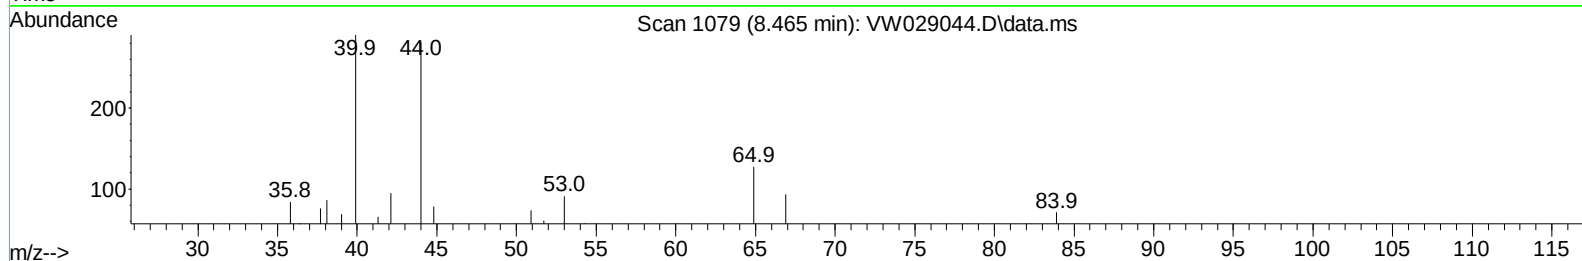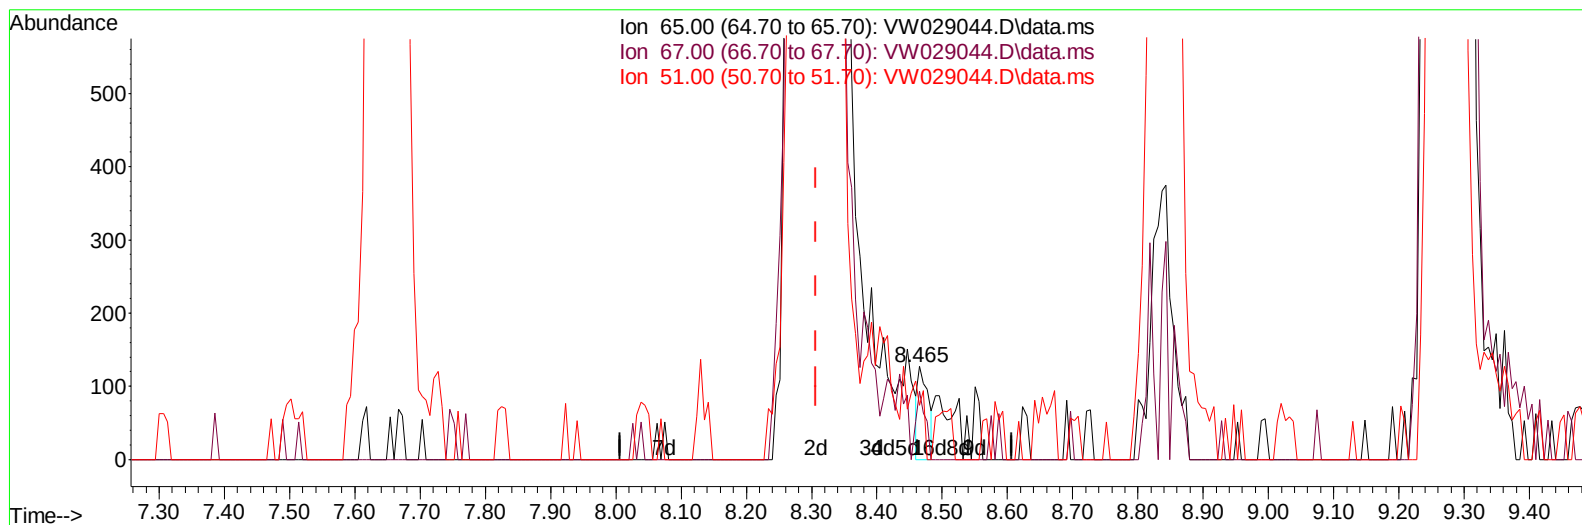

TIC: VW029044.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.465min (+ 0.158) 0.02 ug/L

response 144

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	65.97
51.00	105.10	93.06
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
 Data File : VW029044.D
 Acq On : 06 Jun 2024 17:44
 Operator : SY/MD
 Sample : P2696-08RE
 Misc : 4.43g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BN7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2024
 Supervised By :Mahesh Dadoda 06/07/2024

Quant Time: Jun 07 00:27:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 00:21:46 2024
 Response via : Initial Calibration

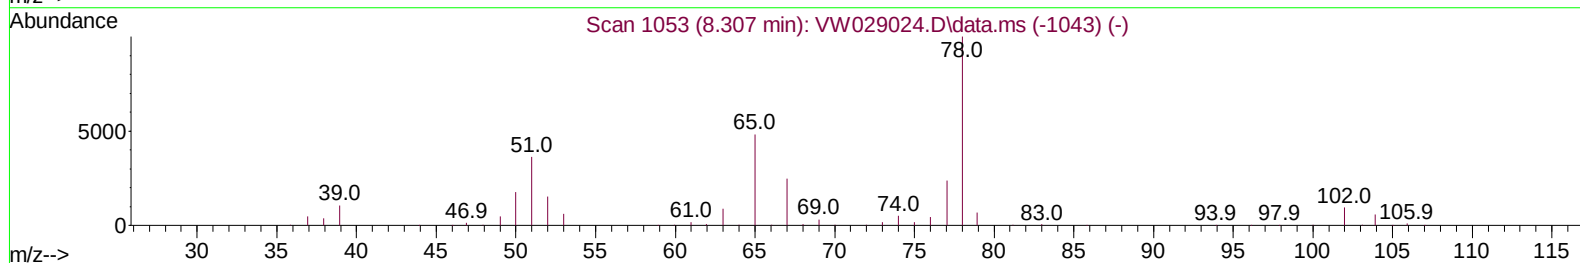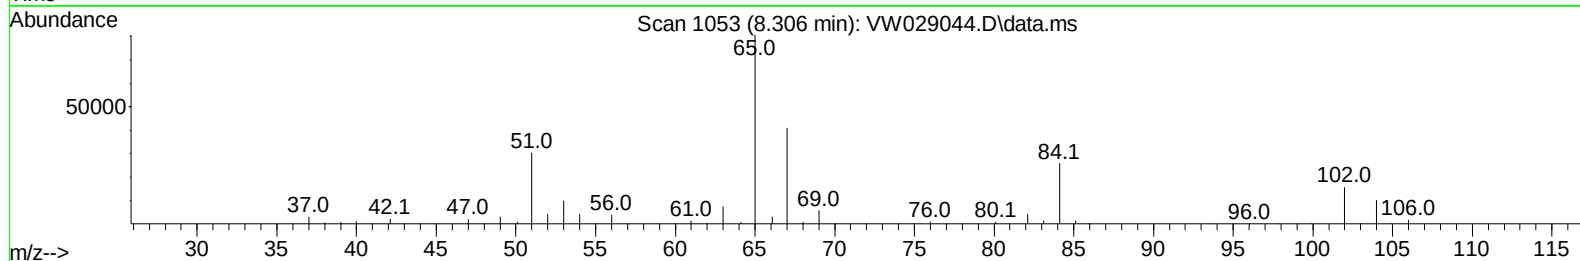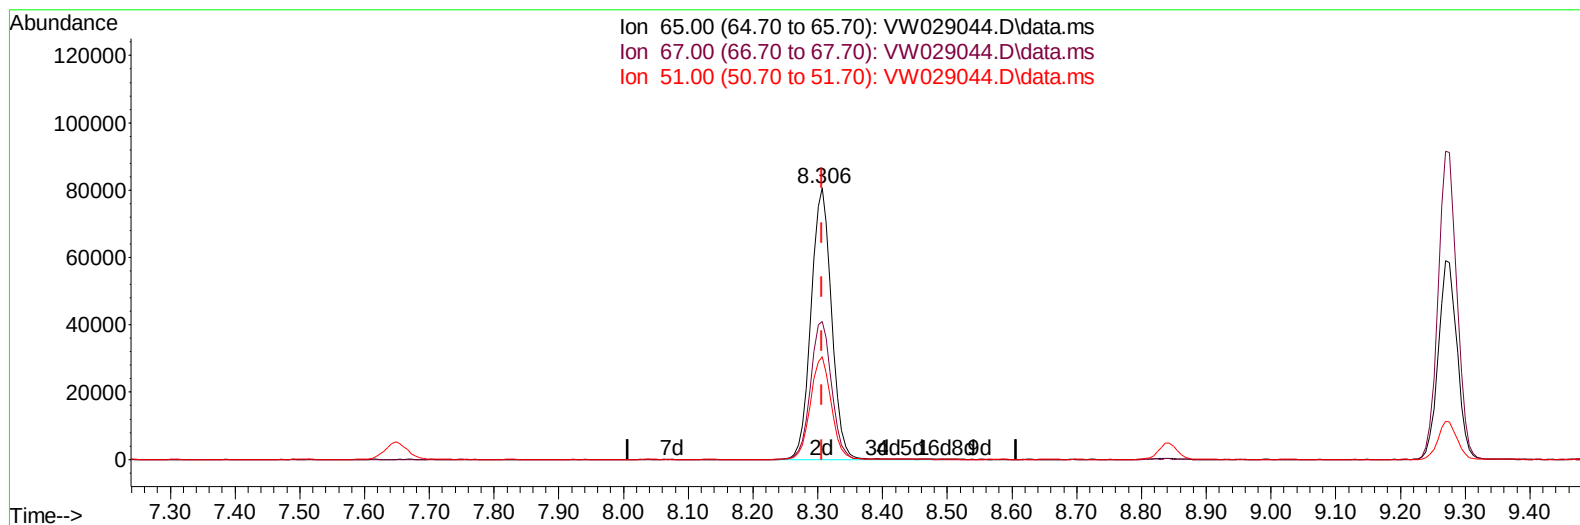

TIC: VW029044.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.306min (-0.000) 26.03 ug/L m

response 177406

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.05#
51.00	105.10	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
 Data File : VW029044.D
 Acq On : 06 Jun 2024 17:44
 Operator : SY/MD
 Sample : P2696-08RE
 Misc : 4.43g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BN7RE

Manual IntegrationsAPPROVED

Quant Time: Jun 07 00:27:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 00:21:46 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/07/2024
 Supervised By :Mahesh Dadoda 06/07/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	453758	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	304218	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	72665	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	162118	22.490	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	89.960%	
7) Chloroethane-d5	2.899	69	132755	23.983	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	95.920%	
11) 1,1-Dichloroethene-d2	4.021	65	67131	21.188	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	84.760%	
21) 2-Butanone-d5	7.075	46	72988	49.557	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	99.120%	
24) Chloroform-d	7.648	84	296539	22.907	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.640%	
26) 1,2-Dichloroethane-d4	8.306	65	177406m	26.031	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	104.120%	
32) Benzene-d6	8.276	84	589708	31.582	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	126.320%	
36) 1,2-Dichloropropane-d6	9.270	67	185096	32.695	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	130.760%#	
41) Toluene-d8	10.318	98	434597	26.082	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	104.320%	
43) trans-1,3-Dichloroprop...	10.574	79	49314	22.669	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.680%	
47) 2-Hexanone-d5	10.922	63	49909	66.804	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	133.600%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	107732	27.392	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	109.560%	
66) 1,2-Dichlorobenzene-d4	13.848	152	57779	22.407	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.640%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
Data File : VW029044.D
Acq On : 06 Jun 2024 17:44
Operator : SY/MD
Sample : P2696-08RE
Misc : 4.43g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BN7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/07/2024
Supervised By :Mahesh Dadoda 06/07/2024

Quant Time: Jun 07 00:27:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 07 00:21:46 2024
Response via : Initial Calibration

