

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
 Data File : VW029030.D
 Acq On : 06 Jun 2024 11:54
 Operator : SY/MD
 Sample : P2696-15
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4DD1

Quant Time: Jun 07 00:23:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 07 00:21:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	303516	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	291938	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	132150	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	101181	20.984	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.920%
7) Chloroethane-d5	2.899	69	78383	21.170	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.680%
11) 1,1-Dichloroethene-d2	4.021	65	44083	20.801	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.200%
21) 2-Butanone-d5	7.075	46	46724	47.428	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.860%
24) Chloroform-d	7.648	84	184323	21.287	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.160%
26) 1,2-Dichloroethane-d4	8.307	65	105710	23.189	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.760%
32) Benzene-d6	8.276	84	372456	20.786	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.160%
36) 1,2-Dichloropropane-d6	9.276	67	116309	21.409	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.640%
41) Toluene-d8	10.318	98	324306	20.282	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.120%
43) trans-1,3-Dichloroprop...	10.575	79	42686	20.447	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.800%
47) 2-Hexanone-d5	10.922	63	32970	45.987	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.980%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	88003	23.317	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	103474	22.065	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.280%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	10502	2.305	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060624\
Data File : VW029030.D
Acq On : 06 Jun 2024 11:54
Operator : SY/MD
Sample : P2696-15
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4DD1

Quant Time: Jun 07 00:23:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060324SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 07 00:21:46 2024
Response via : Initial Calibration

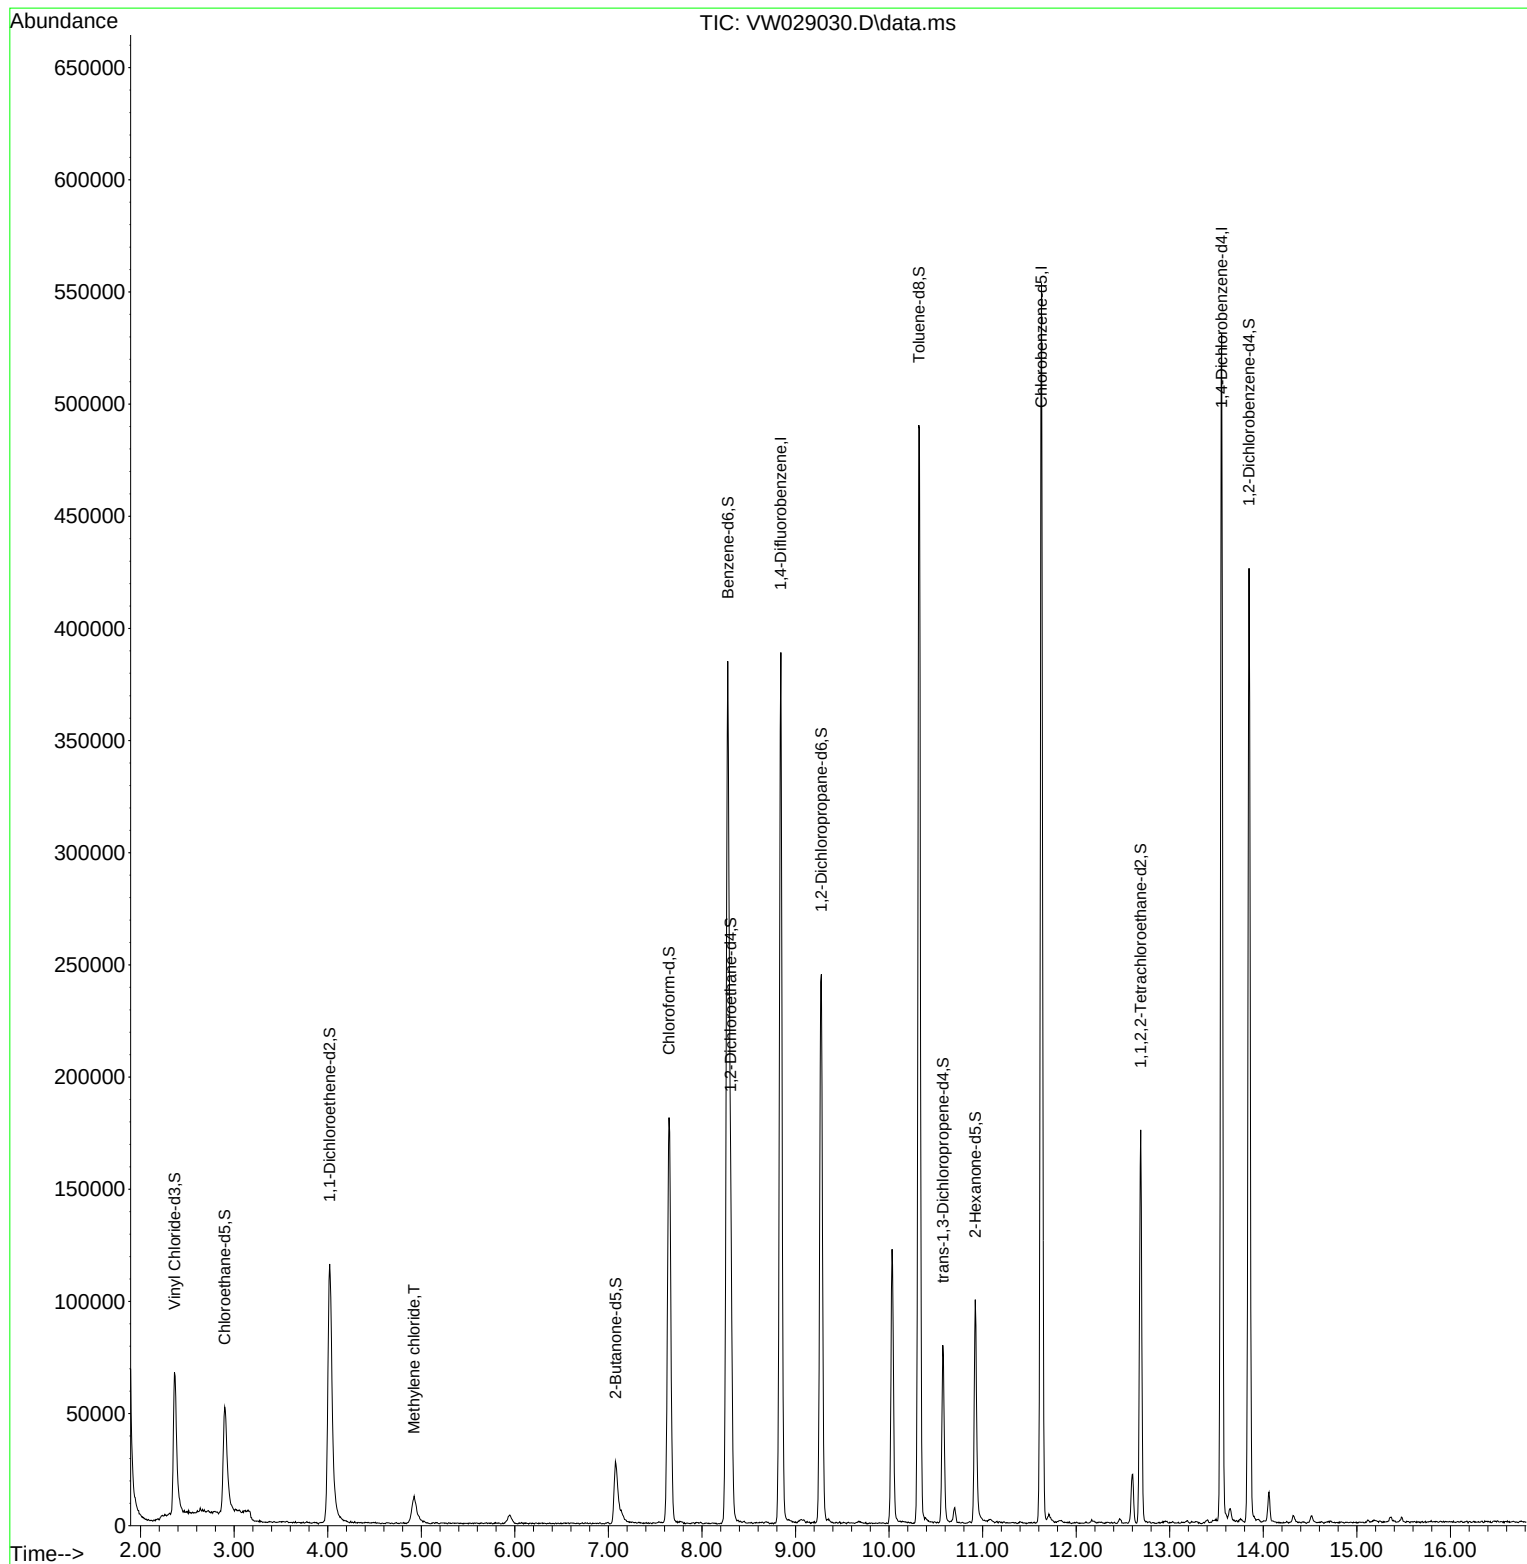

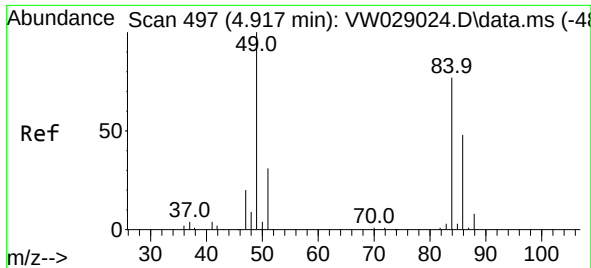

#16
Methylene chloride
Concen: 2.305 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW029030.D
Acq: 06 Jun 2024 11:54

Instrument :
MSVOA_W
ClientSampleId :
A4DD1

Tgt Ion:	84	Resp:	10502
Ion	Ratio	Lower	Upper
84	100		
86	64.1	43.8	81.4
49	133.6	91.3	169.5

